ACCU-CHEK® Insight

Roche

User's Manual

Accu-Chek® Insight Diabetes Therapy System

ACCU-CHEK®

Contents

1 Overview 1

1.1 Understanding Differences When Paired with the Pump 4
1.2 Home Screen 5

2 Startup 9

2.1 Charging the Battery 9
2.2 Setup Wizard 14
2.3 Completing the Setup Wizard 16
2.4 Important Information 22

3 Meter and Pump Communication 31

3.1 Pairing the Meter and Pump 31
3.2 Unpairing the Meter and Pump 38

4 Controlling the Pump with the Meter 41

4.1 Accessing the Pump Menu 42
4.2 Understanding the Pump Menu Screens on the Meter 43
4.3 Stopping the Pump 45
4.4 Starting the Pump 46

5 Testing Your Blood Glucose 47

5.1 Performing a Blood Glucose Test 47
5.2 Adding Information to a Blood Glucose Result 52
5.3 Delivering a Bolus Without Bolus Advice 55

6 Administering Boluses 69

6.1 Programming and Delivering a Standard Bolus 70
6.2 Programming and Delivering an Extended Bolus 72
6.3 Programming and Delivering a Multiwave Bolus 74
6.4 Creating and Delivering a Customised Bolus 76
6.5 Deleting a Customised Bolus 80
6.6 Cancelling a Bolus 82
6.7 Delivering a Bolus Using Bolus Advice 86

7 Temporary Basal Rates 93

7.1 Programming a Basic Temporary Basal Rate (TBR) 93
7.2 Programming or Editing a Customised TBR 95
7.3 Cancelling an Active TBR 98
7.4 Deleting a Customised TBR 100
7.5 Additional TBR Function Information 102

8 Basal Profiles 103

8.1 Programming a Basal Profile 103
8.2 Activating a Basal Profile 107
8.3 Clearing a Basal Profile 109

9 Using Modes 111

9.1 Changing the Signal Mode of the Pump 111
9.2 Turning On Flight Mode 113
9.3 Turning Off Flight Mode 114

10 Pump Settings 115

10.1 Pump Reminders 116
10.2 Therapy Settings 127
10.3 Device Settings 141
10.4 Setting the Pump Date and Time 150

11 My Data 153

11.1 Overview 153
11.2 The Logbook 154
11.3 The Trend Graph 170
11.4 The Standard Week 176
11.5 The Standard Day 182
11.6 Target Data 188
11.7 The bG Averages Table 193

12 Technical Information 199

12.1 Explanation of Symbols 200
12.2 List of Icons 201

13 Troubleshooting 205

14 Glossary 209

Index 223

1 Overview

With the Accu-Chek Aviva Insight diabetes manager (hereafter referred to as the meter), you can remotely control the Accu-Chek Insight insulin pump using *Bluetooth*® wireless technology.

If you experience any communication problems between the pump and meter, operate the pump manually.

With the meter, you can remotely control the following pump functions:

- Delivering boluses
- Setting basal rates
- Starting and stopping the pump
- Changing pump modes
- Changing pump settings
- Setting pump reminders

With the meter, you cannot remotely control the following pump functions:

- Changing the cartridge
- Priming the infusion set
- Rewinding the piston rod
- Controlling settings within the Bluetooth wireless technology menu on the pump
- Changing the pump display settings
- Selecting user profiles

NOTE

- When the meter and pump are connected, you can still program and deliver a bolus manually with the pump without using the meter's commands.
- When the meter and pump are connected, the pump automatically transfers bolus information to the meter.
- If bolus advice is set up, it is important that you enter carbohydrate information and/or health events into the meter for boluses you have delivered manually on the pump so that future bolus advice recommendations are appropriate.
- The pump display must be off in order for the meter to connect to the pump.
- If you unlock the keys on your pump while Bluetooth communication is active, the pump asks if you would like to disconnect the Bluetooth connection. Select "no" to keep the Bluetooth connection intact and continue operating your pump through the meter. Select "yes" to disconnect and operate the pump using the pump display.
- You can cancel any bolus that is being delivered by the pump either by manually using the pump or remotely through the Pump Menu on the meter.

NOTE

- The meter and pump can communicate within a 2 metre range.
- When the meter and pump are communicating, the meter displays maintenance screens that would otherwise display on the pump. When a pump maintenance screen displays on the meter, press OK to acknowledge and dismiss the message. You must still take any actions recommended by the maintenance message.

1.1 Understanding Differences When Paired with the Pump

If you have used the meter or pump on its own before pairing, you should be aware that the paired system behaves differently as follows:

- Bolus advice can be used to immediately deliver the recommended bolus.
- When the meter calculates bolus advice, the maximum bolus value is taken from pump settings.
- Boluses can be adjusted by much smaller amounts. For boluses of 10 units or more, the insulin increment is 0.1 U. For boluses of less than 10 units, the insulin increment is 0.05 U. This also applies to manually-entered bolus information in new logbook records.
- Because insulin increment and maximum bolus settings are taken from the pump, these settings are not available in the meter settings menu.
- Basal appears on the Pump Menu and not the Bolus Input or Detailed bG Result screen.
- The Basal Injection reminder is no longer available.
- Basal no longer appears when manually entering logbook records.

1.2 Home Screen

Home screen refers to the screen that is displayed when the meter is powered on. Home screen can be either the Main Menu or Status screen. To change the Home screen default, see the **Home Screen Default** section in the **Changing Meter Settings** chapter of the **Accu-Chek Aviva Insight Diabetes Manager User's Manual**.

1.2.1 Main Menu Screen

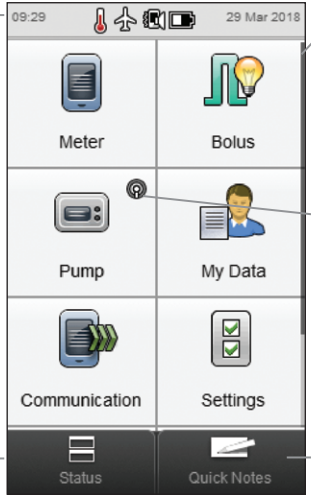

Title Bar
Displays meter information.

Menu Selections

Go to Status Screen
See the **Status Screen** section in this chapter.

Scroll Bar
Appears when there is more information than fits on the screen.

Pump Communication Icon
Appears when the meter and pump are communicating.

Go to Quick Notes Screen

The **Title Bar** shows the time of day and date. For explanations of the icons that are displayed in the **Title Bar**, see the **Understanding Your Diabetes Manager** chapter of the **Accu-Chek Aviva Insight Diabetes Manager User's Manual**.

1.2.2 Status Screen

When the meter is paired with the pump, the Status screen displays the pump status, as well as information for the most recent valid blood glucose test.

For a detailed description of the bG Status portion of the Status screen, refer to the **Understanding Your Diabetes Manager** chapter of the **Accu-Chek Aviva Insight Diabetes Manager User's Manual**.

To view a fullscreen version of either the Pump Status or bG Status, touch that portion of the Status screen.

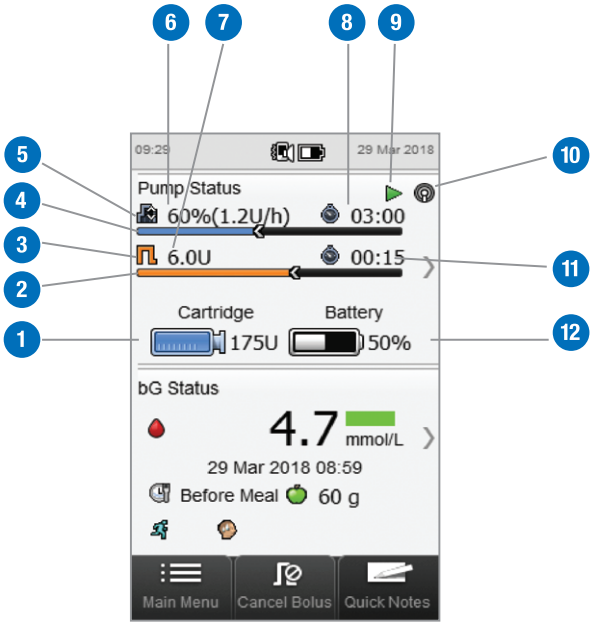

1	**Cartridge level** Shows units of insulin remaining in the cartridge.
2	**Bolus progress bar** Visually represents amount and duration of the active bolus (not visible if no bolus is being delivered).
3	**Bolus type icon** Indicates bolus type of the active bolus.
4	**TBR progress bar** Visually represents amount and duration of the active temporary basal rate.
5	**Basal icon** Indicates an active basal profile or temporary basal rate (TBR).
6	**Basal rate** Shows basal rate in units per hour (U/h). For temporary basal rates, also shows percentage value of the active basal profile time block.
7	**Bolus insulin remaining** Shows units of bolus insulin remaining of the active bolus.
8	**TBR time remaining** Shows the time remaining of the active temporary basal rate.
9	**Pump status** Indicates whether the pump is running or is stopped.
10	**Communication icon** Indicates that the meter and pump are communicating.
11	**Bolus time remaining** Shows amount of time remaining of an extended or multiwave bolus.
12	**Pump battery level** Shows remaining charge of pump battery.

2 Startup

2.1 Charging the Battery

Charge the battery by plugging the USB cable into either a power outlet or a computer. Use the USB cable and USB power adapter supplied with the meter to avoid problems when charging the battery. The preferred charging method is to use a power outlet since this is faster and takes about 3.5 hours to charge a fully drained battery. Charging the meter from a computer takes much longer. Use a power outlet if the battery is extremely low on power or has not been charged for a while.

NOTE

- Allowing the battery to fully drain reduces the ability of the battery to hold its charge. It is recommended that you recharge the battery on a regular basis, for example once every day. Keeping the meter plugged in to charge does not harm the battery.
- A blood glucose test cannot be performed while the meter is plugged in.

Charging the Battery Using a Power Outlet

1

If the power adapter is already assembled, proceed to Step 4. To assemble the power adapter, remove the clear plastic cover by pressing the centre of the release button. Slide the clear plastic cover off in the direction of the arrow.

2

Slide on the pronged plug where the clear plastic cover was located until it firmly clicks into place. Do not try to force the pronged plug. It only goes on one way.

3

Plug the larger end of the USB cable into the power adapter.

4

Plug the smaller end of the USB cable into the meter.

5

Plug the power adapter into a power outlet. If the battery is extremely low on power, the meter does not turn on for a number of minutes.

When the connection is successful, the meter displays the battery charging screen for 3 seconds.

The next screen (either the Main Menu or Status screen) displays the battery icon in charging mode.

6

When the battery icon is shown as fully charged, you can unplug the meter.

Charging the Battery Using a Computer

1

Plug the smaller end of the USB cable into the meter.

2

Plug the larger end of the USB cable into an available USB port on the PC. If the battery is extremely low on power, the meter does not turn on. Charge the battery using a power outlet.

3

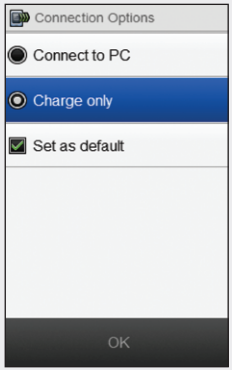

Choose Charge only. As an option, choose Set as default to keep this screen from appearing each time you connect the USB cable to a PC. Select OK.

NOTE

- The Connection Options screen does not appear if Set as default was chosen previously.
- To remove the default, go to the Main Menu and select Communication > Settings. Choose Prompt upon USB connect. Select Save.

NOTE

The PC must be turned on and not in sleep or standby mode to charge the battery.

When the connection is successful, the meter displays the battery charging screen for 3 seconds.

The next screen (either the Main Menu or Status screen) displays the battery icon in charging mode.

NOTE

The computer is not charging the battery if the meter does not display the battery charging screen or the battery charging icon, or if the Information screen Recharge meter soon is displayed. Charge the battery using a power outlet.

4

When the battery icon is shown as fully charged, you can unplug the meter.

2.2 Setup Wizard

The first time you turn the meter on, the Setup Wizard is activated. You must complete the Setup Wizard before performing a blood glucose test for the first time.

The Setup Wizard assists you in selecting settings for:

- Meter language
- Time and date
- Units (carbohydrate)
- Warning limits for hypo (low) and hyper (high) blood glucose levels
- Time blocks
- Bolus advice (optional)
- bG test reminders (optional)

⚠ WARNING

It is important to discuss your individual settings for warning limits, time blocks, bolus advice and bG test reminders with your healthcare professional.

NOTE

- The Setup Wizard is activated every time you turn the meter on until you complete the process.
- If you turn the meter off during the Setup Wizard, you must reconfirm all of the settings in order to complete the Setup Wizard.
- To return to a previous screen in the Setup Wizard, select Back.
- If you choose not to set up bolus advice and bG test reminders as part of the Setup Wizard, these features can be set up later. For information on how to set up these features after completion of the Setup Wizard, see **Setting Up Bolus Advice** under the **Changing Bolus Advice Settings** chapter of the **Accu-Chek Aviva Insight Diabetes Manager User's Manual**.
- The default settings in the meter and the settings illustrated in this User's Manual are for example only.

2.3 Completing the Setup Wizard

Refer to the **Important Information** section of this User's Manual for detailed explanations of the various settings in the Setup Wizard.

1

Starting with the meter turned off, press the power button to turn on the meter.

2

The meter vibrates, beeps and displays this splash screen for a short period of time (this screen appears each time the meter is turned on).

3

Choose the desired language from the list. Select Next.

4

If you are using the Accu-Chek 360° configuration software: Plug the meter into the PC, choose PC setup, and then select Next to continue the setup using the software. You do not need to follow the rest of the steps in this section.



To proceed with setup on the meter, choose Manual. Select Next.

5



Select 12 hr or 24 hr to set the time format, if necessary.

6



Set the date and time. Select Next.

7



Choose the appropriate carbohydrate unit. Select Next.

8



Set the Hyper (upper) and Hypo (lower) warning limits. Select Next.

9



Choose Yes to receive bolus advice. Choose No to not receive bolus advice. Select Next.

10



Set the start time and end time for the first time block. Select Next.

11

Set the target range. Select Next.

NOTE

If you choose not to receive bolus advice, the Setup Wizard skips Step 12.

12



Set the Carbohydrate ratio and Insulin sensitivity. Select Next.

13



Select OK.

14



Select any additional time block to edit the End time, Upper value and Lower value. Select Next when you have finished editing the time blocks.

NOTE

- If bolus advice is on, you can also set the carbohydrate ratio and insulin sensitivity for each time block.
- To reset all edited time blocks to their default values, select Cancel and then Yes. This restarts the meter setup process.
- If you chose not to receive bolus advice, Done appears instead of Next on the screen. Select Done to complete the Setup Wizard.

15



Set the percentage for any desired health events. Scroll to view additional options. Select Next.

16

Set the Meal rise, Snack size, Acting time and Offset time. Select Done to complete the Setup Wizard.

NOTE

Consult your healthcare professional and read the **Bolus Advice** chapter of the **Accu-Chek Aviva Insight Diabetes Manager User's Manual** for help with any of the settings in the Setup Wizard.

2.4 Important Information

2.4.1 Carbohydrate Unit

You have a choice among different carbohydrate units in the meter that best fit your needs. The following carbohydrate units are available:

Abbreviation	Unit of Measurement	Gram Equivalent
g	Grams	1 gram
KE	Kohlenhydrateinheit (Carbohydrate Unit)	10 grams
BE	Bread Equivalent	12 grams
CC	Carbohydrate Choice	15 grams

NOTE

The gram equivalents for KE, BE and CC can be changed using the Accu-Chek 360° configuration software. The default gram equivalents are shown in the previous table.

2.4.2 Warning Limits

You can select hyper (high) and hypo (low) blood glucose warning limits that best fit your needs.

Whenever a blood glucose result is above the hyper warning limit or below the hypo warning limit, the meter displays a warning.

- Set the hyper warning limit greater than the target range of all time blocks.
- Set the hypo warning limit less than the target range of all time blocks.

2.4.3 Time Blocks

Setting time blocks to fit your own schedule helps you and your healthcare professional see how patterns in your blood glucose levels may be affected by your daily activities and lifestyle.

Time blocks combine to cover a 24-hour time period.

The meter comes with four default time blocks. You may set up to eight time blocks. You can change the time period for any of the default time blocks.

To complete the Setup Wizard, you must complete and save the default settings for the time blocks. Each time block must be at least 15 minutes long and can only be set in 15-minute increments. When you set the end time for a time block, the meter automatically sets this end time as the start time for the next time block.

You can set a different blood glucose target range for each time block. The target range for each time block must be within the hypo and hyper warning limits.

When the default time blocks are set up, the settings are applied to all of the other time blocks. If bolus advice is set up, you must also set the carbohydrate ratio and insulin sensitivity for the default time block. You can set a different carbohydrate ratio and insulin sensitivity for each time block.

Talk to your healthcare professional about setting up time blocks.

2.4.4 Bolus Advice

The bolus advice feature calculates a bolus for you that is customised to the time of day and your changing situations. This function is activated only if you set up bolus advice on your meter.

Bolus advice recommendations provided by the meter are intended solely as advice.

For more detailed information on bolus advice, see the **Bolus Advice** chapter of the **Accu-Chek Aviva Insight Diabetes Manager User's Manual**.

Carbohydrate Ratio

The carbohydrate ratio is the amount of insulin necessary to account for a certain amount of carbohydrates.

Talk to your healthcare professional to determine the appropriate carbohydrate ratio for you.

Insulin Sensitivity

The insulin sensitivity is the amount of insulin necessary to lower your blood glucose by a certain amount.

Talk to your healthcare professional to determine the appropriate insulin sensitivity settings for you.

Health Events

Health events can be selected to indicate how you are feeling or what you are doing that might affect your blood glucose level. You have the option of setting a percentage for each health event which adjusts the bolus advice recommendation.

Health events available on the meter are:

- Exercise 1
- Exercise 2
- Stress
- Illness
- Premenstrual
- Customized (1–3)

A positive percentage increases the bolus amount and a negative percentage (-) decreases the bolus amount. Talk to your healthcare professional to determine the appropriate percentage for each health event for you.

Advice Options

Meal rise, snack size, acting time and offset time are advice options. Below are detailed descriptions of each of these settings.

Meal Rise

During or after meals, an increase in blood glucose level is considered normal within a certain range, even though a bolus has been delivered.

Enter the maximum increase in your blood glucose level that is to be tolerated after a meal without an additional correction bolus.

Snack Size

The snack size defines a threshold of carbohydrates above which a meal rise is triggered.

Acting Time

The period of time from the start of bolus until your blood glucose level is expected to return to the target level.

You can adjust the length of the acting time to fit your individual needs within a specified time interval (1 ½ hours to 8 hours). If you are unsure of your insulin acting time, check with your healthcare professional.

The total acting time includes the offset time.

Offset Time

Offset time is the expected amount of time before the insulin begins to lower blood glucose levels in the body.

3 Meter and Pump Communication

3.1 Pairing the Meter and Pump

Before you can control the pump with the meter, the meter and pump must be paired. If you received the meter and pump as a kit, they come paired by default.

Once the meter and pump are paired, the pairing settings are stored in both devices so that you do not have to repeat the pairing. If communication between the meter and pump is stopped or interrupted for any reason, they will automatically resume communication whenever both devices are in communication range and the pump display is not active.

Main Menu > Communication > Set Up New Pairing > Devices

1



From the meter's Main Menu, select Communication.

2



Select Set Up New Pairing.

The meter displays the Prepare Device screen.

3

On the pump, select Settings.

4

Select Communication.

5

Select Add device.



The pump displays the Add device screen showing the serial number of the pump.

6

On the meter, select Next.



The meter displays the Searching screen while it searches for discoverable Bluetooth devices.

NOTE

- The meter can only be paired with one pump at a time. If either device was previously paired to another device (for instance, if this is a replacement meter or pump), you must first remove the previous pairing. See the **Unpairing the Meter and Pump** section of this chapter for instructions on unpairing your devices.
- When in Add device mode, the pump sends a signal that other devices can detect in order to pair with the pump.
- For more detailed instructions on how to set the pump to Add device mode, refer to the **Accu-Chek Insight Insulin Pump User's Manual**.

7

Select the serial number that matches the one displayed on the pump screen from the list.

The meter attempts to pair with the pump and displays the Pairing screen.



The pump displays the Add device screen.

8



Verify that the PIN code on the meter matches the one displayed on the pump screen. Select Yes on the meter.



Confirm on the pump.

NOTE

- If the PIN code and serial number do not match what is displayed on the device you intend to pair with the meter, select No.
- If the meter is unable to pair with the device selected, the Device Not Paired screen appears. Select OK to return to the Communication menu.

9



Select OK.

NOTE

- Bluetooth wireless communication must be turned on and the meter be connected to the pump in order to perform pump functions using the meter.
- When your meter is paired with the pump, the default home screen of the meter is changed from the Main Menu to the Status screen. For information on the Status screen, refer to the **Home Screen** section of the **Overview** chapter of this User's Manual.
- If communication is lost between the meter and pump and an error occurs on the pump, the error message is not displayed on the meter. If you turn the meter on and reconnect to the pump, the error message is displayed on the meter.

3.2 Unpairing the Meter and Pump

Main Menu > Communication > Manage Current Pairings

1



From the Main Menu, select Communication.

2



Select Manage Current Pairings.

3



Select ✕ next to the name of the pump.

4



Select Yes.

NOTE

This process deletes the pairing on the meter and ends communication between the meter and pump. For instructions on deleting the pairing information on the pump, refer to the **Accu-Chek Insight Insulin Pump User's Manual**.

4 Controlling the Pump with the Meter

⚠ WARNING

Check your blood glucose level and replace the missing insulin immediately if your insulin delivery is interrupted for any reason.

For example:

- You stop the pump.
- There is a technical problem with the pump.
- The cartridge and/or the infusion set is leaking.
- There is an occlusion in the infusion set.
- The cannula has slipped out of the infusion set.

⚠ WARNING

If communication between the pump and meter is interrupted or is no longer possible for any reason, the meter displays the **M-68 Connection Lost** maintenance message. In this event, use the pump as a standalone device.

4.1 Accessing the Pump Menu

When the meter is paired with the pump, a number of remote features are enabled on the meter which were not previously available. You can access these features from the Pump Menu.

Main Menu > Pump

1



From the Main Menu, select Pump.

4.2 Understanding the Pump Menu Screens on the Meter

The Pump Menu contains the following options:



Menu Option	Description
Bolus	Program and deliver boluses, as well as create and modify customised boluses
Basal	Program, create and modify temporary basal rates (TBR), as well as program and activate basal profiles
Stop pump	Stop insulin delivery
Start pump	Start insulin delivery
Pump Data	View reports on Event, Bolus and TBR data, as well as Daily Totals, Pump Timer and Software Version information
Modes	Adjust signal modes and turn Flight Mode on and off
Settings	Program Pump Reminders, and access Device, Therapy, and Time and Date settings

Icon	Description
Pump Stopped icon	Indicates pump has stopped. Pump Running and Pump Paused icons can also appear here
Pump Running icon	(Not shown) Indicates pump is running
Pump Paused icon	(Not shown) Indicates pump has been paused

NOTE

If your pump has a warning or error while communicating with your meter, the warning or error message displays on the meter. Pressing OK on the meter message screen dismisses the warning/error on both devices. You must still perform any actions recommended by the message; pressing OK does not perform these actions automatically.

4.3 Stopping the Pump

Main Menu > Pump > Stop Pump

1



From the Pump Menu, select Stop pump. This stops insulin delivery from the pump.

2



Select Yes.

3



The meter displays the Status screen, which shows that the pump has stopped.

4.4 Starting the Pump

Main Menu > Pump > Start Pump

1



From the Pump Menu, select Start pump. This starts insulin delivery from the pump.

2



Select Yes.

3



The meter displays the Status screen, which shows that the pump has started.

5 Testing Your Blood Glucose

5.1 Performing a Blood Glucose Test

NOTE

- You need the meter, a test strip, a lancing device and a lancet.
- Set up the meter before you perform your first blood glucose test.
- A blood glucose test cannot be performed while the meter is plugged in.
- Blood glucose is sometimes shortened to bG, but it means the same thing.

1



Wash and dry your hands. Prepare the lancing device.

2

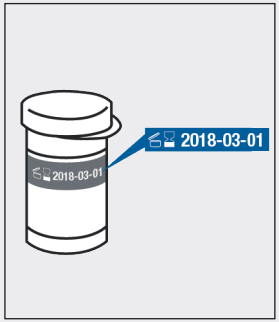

Check the use by date on the test strip container. Do not use test strips past the use by date.

3

Insert the test strip into the meter in the direction of the arrows. The meter turns on.

NOTE

- Do not touch the blood drop to the test strip until the Apply Drop screen is displayed.
- Be careful not to put any fluids into the test strip slot.
- If a test strip error occurs, remove and discard the test strip. Repeat the test with a new test strip.
- Do not apply a blood drop to the test strip before you insert it into the meter.
- When a test strip is in the meter, the buttons and touchscreen selections are inactive, including the power button. The buttons become active when you remove the test strip or when the test is complete.
- Other ways to start a blood glucose test:
  - From the Main Menu, select Meter > bG Test or select Bolus > bG Test. Insert a test strip into the meter.
  - When a bG test reminder notification is displayed, insert a test strip into the meter.

An image of the test strip container is displayed for a few seconds. Continue to the next step.

4



The Apply Drop screen appears. Perform a finger prick with the lancing device.

5



Gently squeeze your finger to assist the flow of blood. This helps you get a blood drop.

6



Touch the blood drop to the **front edge** of the yellow window of the test strip. Do not put blood on top of the test strip.

The Analyzing screen appears when there is enough blood in the test strip.

The result appears on the display.

NOTE

- For information about blood glucose results, see the **Understanding Blood Glucose Results** and **Unusual Blood Glucose Results** sections in the **Accu-Chek Aviva Insight Diabetes Manager User's Manual**.
- The blood glucose result must be used within 10 minutes for bolus advice.

7



In approximately 3 seconds the Detailed bG Result screen appears. Remove and discard the used test strip. Perform one of the following:

- Complete the blood glucose test without adding information or delivering a bolus: Select Done.

- If bolus advice is enabled: Go to the **Delivering a Bolus Using Bolus Advice** section in the **Administering Boluses** chapter in this User's Manual.

- If bolus advice is not enabled:
  - Add information to be saved with the blood glucose result: Continue to the next section **Adding Information to a Blood Glucose Result**. A bolus can be delivered after adding the information.
  - Deliver a bolus without adding information: Select Bolus and go to the **Delivering a Bolus Without Bolus Advice** section in this chapter.

5.2 Adding Information to a Blood Glucose Result

Adding information to the entry fields provides you with a record of the circumstances surrounding your blood glucose result. This information is helpful later for determining patterns in your blood glucose levels. The steps in this section only apply if the bolus advice feature is not being used. If bolus advice is enabled, go to the **Delivering a Bolus Using Bolus Advice** section in the **Administering Boluses** chapter in this User's Manual.

1



To add an entry, select it and refer to the instructions on the following page.

Screens for Adding Entries for Detailed bG Result

Meal Time



Choose the meal time. Select Save.

Carbohydrates



Set the number of carbohydrates consumed. Select Save.

Health Events



Choose up to four health events. Select Save.

NOTE

If bolus advice is turned on, and multiple health events have been chosen, the Adjustment screen on the meter displays “---%”. You must enter a summarised health event percentage, even if this percentage is zero.

Note

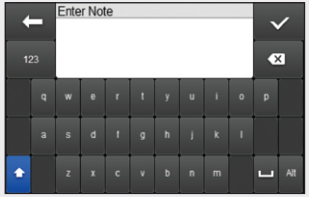

Type a note (up to 60 characters) to save with this record. Select ✓.

2



Perform one of the following:

- Save the entries and proceed with bolus delivery: Select Bolus and continue.
- Save the entries and do not proceed with bolus delivery: Select Done.

5.3 Delivering a Bolus Without Bolus Advice

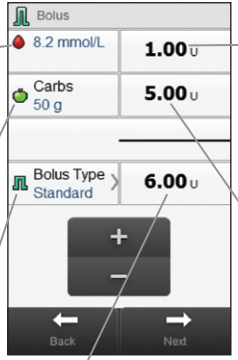

bG Result
No bG Test is displayed if 10 minutes or more have elapsed since the last bG result was obtained.

Carbohydrate Amount
No Entry is displayed if no amount is entered.

Bolus Type
See the following table.

Total Bolus
Sum of the Correction Bolus and Carbohydrate Bolus amounts.

Correction Bolus
Insulin to return an out-of-target blood glucose to a target value.

Carbohydrate Bolus
Insulin to account for the food you eat.

NOTE

When the Bolus screen first appears, there are no bolus amounts. The bolus amounts are entered by you.

Bolus Type

When programming a bolus without using bolus advice, the default bolus type displayed on the meter varies depending on the state of communication with the pump.

Condition	Bolus Type
The meter is communicating with the pump and the Standard Bolus is available from the pump.	The bolus type is initially set to Standard. You are able to change the bolus type.
The meter is communicating with the pump and the Standard Bolus is not available from the pump.	The bolus type is initially set to Manual on Pump. You are able to change the bolus type.
The meter is paired to a pump and not communicating with the pump.	The bolus type is initially set to Manual on Pump. You are able to change the bolus type.
The meter is paired to a pump and communicating with the pump, but the pump is paused or stopped.	The bolus type is initially set to Pen/Syringe. You are able to change the bolus type.
The meter is not paired with a pump.	The bolus type button is not displayed. The bolus type is set to Pen/Syringe and cannot be changed.

5.3.1 Delivering a Standard Bolus Without Bolus Advice

1



If necessary, change to Standard bolus by selecting Bolus Type. Otherwise, proceed to Step 3.

2



Choose Standard. Select Save.

3



Enter the bolus amounts, as necessary. To input a bolus amount, select the entry field for Correction Bolus, Carbohydrate Bolus or Total Bolus and set the amount.

NOTE

- If you set either the Correction Bolus or the Carbohydrate Bolus first: The ability to edit the Total Bolus is disabled; however, the Total Bolus updates accordingly.
- If you set the Total Bolus first: The ability to edit the Correction Bolus and Carbohydrate Bolus is disabled; however, the Correction Bolus updates accordingly.

4



Select Next.

5



Select Next.

6



Select Back to adjust the bolus, or select OK to deliver the bolus.



The pump delivers the bolus and the meter displays the Status screen showing the current bolus information.

5.3.2 Delivering an Extended Bolus Without Bolus Advice

1



Select Bolus Type.

2



Choose Extended. Select Save.

NOTE

The Extended Bolus is available only if a Carbohydrate Bolus is entered.

3

Enter the bolus amounts as necessary. To input the bolus amount, select the entry field for Correction Bolus, Carbohydrate Bolus or Total Bolus, and set the amount.

4



Select Next.

5



Set delayed duration. Select Next.

6



Select Back to adjust a setting, or select OK to deliver the bolus.



The pump delivers the bolus and the meter displays the Status screen showing the current bolus information.

5.3.3 Delivering a Multiwave Bolus Without Bolus Advice

1



Enter the bolus amounts, as necessary. To input a bolus amount, select the entry field for Correction Bolus, Carbohydrate Bolus or Total Bolus, and set the amount.

2



Select Bolus Type.

NOTE

The Multiwave Bolus is only available if a Carbohydrate Bolus is entered.

3



Choose Multiwave. Select Save.

NOTE

- If you set either the Correction Bolus or the Carbohydrate Bolus first: The ability to edit the Total Bolus is disabled; however, the Total Bolus updates accordingly.
- If you set the Total Bolus first: The ability to edit the Correction Bolus and Carbohydrate Bolus is disabled; however, the Correction Bolus updates accordingly.
- If a Carbohydrate Bolus is entered and no amount has been entered for carbohydrates (Carbs displays No Entry in Step 2), you should consider entering an amount for carbohydrates. Select Back to enter an amount. An amount is not required, but the more complete the data the more accurate any future bolus advice recommendations are when using bolus advice.

4



Select Next.

5



Set the immediate amount, delayed amount and delayed duration. Select Next.

6

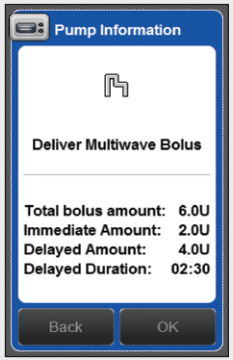

Select Back to adjust a setting, or select OK to deliver the bolus.



The pump delivers the bolus and the meter displays the Status screen showing the current bolus information.

5.3.4 Delivering a Pen/Syringe Bolus Without Bolus Advice

1



If necessary, change to Pen/Syringe bolus by selecting Bolus Type. Otherwise, proceed to Step 3.

2



Choose Pen/Syringe. Select Save.

3



Enter the bolus amounts, as necessary. To input a bolus amount, select the entry field for Correction Bolus, Carbohydrate Bolus or Total Bolus, and set the amount.

NOTE

- If you set either the Correction Bolus or the Carbohydrate Bolus first: The ability to edit the Total Bolus is disabled; however, the Total Bolus updates accordingly.
- If you set the Total Bolus first: The ability to edit the Correction Bolus and Carbohydrate Bolus is disabled; however, the Correction Bolus updates accordingly.

4



Select Next.

5



Select Back to adjust the bolus amount, or select OK. Deliver the bolus using your pen or syringe.

5.3.5 Delivering a Manual on Pump Bolus Without Bolus Advice

1



If necessary, change to Manual on Pump bolus by selecting Bolus Type. Otherwise, proceed to Step 3.

2



Choose Manual on Pump. Select Save.

3



Enter the bolus amounts, as necessary. To input a bolus amount, select the entry field for Correction Bolus, Carbohydrate Bolus or Total Bolus, and set the amount.

NOTE

- If you set either the Correction Bolus or the Carbohydrate Bolus first: The ability to edit the Total Bolus is disabled; however, the Total Bolus updates accordingly.
- If you set the Total Bolus first: The ability to edit the Correction Bolus and Carbohydrate Bolus is disabled; however, the Correction Bolus updates accordingly.

4



Select Next.

5



Select Back to adjust the bolus amount, or select OK to record the bolus. Program the pump to deliver the bolus.

6 Administering Boluses

NOTE

- Refer to the **Accu-Chek Insight Insulin Pump User's Manual** for a detailed explanation of standard, extended and multiwave boluses.
- Lag time-related features only appear on the meter if you have enabled lag time on the pump.

6.1 Programming and Delivering a Standard Bolus

Main Menu > Pump > Bolus > Standard Bolus

1



From the Pump Menu, select Bolus.

2



Select Standard Bolus.

3



Set the immediate amount.
Select Next.

4



Select OK.

NOTE

Selecting Back takes you back to the previous screen without delivering a bolus.

5



The pump delivers the bolus and the meter displays the Status screen showing the current bolus information.

6.2 Programming and Delivering an Extended Bolus

Main Menu > Pump > Bolus > Extended Bolus

1



From the Pump Menu, select Bolus.

2



Select Extended Bolus.

3



Set the delayed amount and delayed duration. Select Next.

4



Select OK.

NOTE

Selecting Back takes you back to the previous screen without delivering a bolus.

5



The pump delivers the bolus and the meter displays the Status screen showing the current bolus information.

6.3 Programming and Delivering a Multiwave Bolus

Main Menu > Pump > Bolus > Multiwave Bolus

1



From the Pump Menu, select Bolus.

2



Select Multiwave Bolus.

3



Set the immediate amount, delayed amount and delayed duration. Select Next.

4



Select OK.

NOTE

Selecting Back takes you back to the previous screen without delivering a bolus.

5



The pump delivers the bolus and the meter displays the Status screen showing the current bolus information.

6.4 Creating and Delivering a Customised Bolus

Main Menu > Pump > Bolus > Customized Bolus

NOTE

- If you have enabled the lag time feature on the pump, you can adjust the lag time for each bolus type when creating a customised bolus.
- When set, lag time is only applied to the current bolus delivery and is not saved with the other settings of a customised bolus.

1



From the Pump Menu, select Bolus.

2



Select ⊕ New Bolus.

3



Select the bolus type for the customised bolus (Standard, Extended or Multiwave).

4



Change the settings for the selected bolus type.

Bolus Type	Settings
Customized Standard Bolus	Set immediate amount.
Customized Extended Bolus	Set delayed amount and Set delayed duration.
Customized Multiwave Bolus	Set immediate amount, Set delayed amount and Set delayed duration.

5



Select Edit Name.

6

Type the name you wish to use for the customised bolus. Select ✓.

7



Select Next to deliver the bolus, or Save to save the bolus for future use without delivering immediately.

NOTE

- Selecting Back takes you back to the previous screen without delivering a bolus.
- Saved customised boluses appear in the list of available boluses in the Bolus menu and on the pump.

8

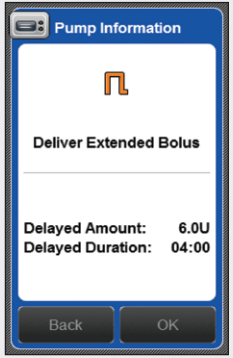

Select OK to deliver the bolus.

9



The pump delivers the bolus and the meter displays the Status screen showing the current bolus information.

6.5 Deleting a Customised Bolus

Main Menu > Pump > Bolus

1



From the Pump Menu, select Bolus.

2



Select ✕ next to the customised bolus you wish to delete.

3


Pump Information
Favorite meal
This bolus will be deleted.
Back
OK

Select OK.

6.6 Cancelling a Bolus

6.6.1 Cancelling a Bolus from the Status Screen

Main Menu > Status

1



From the Main Menu, select Status.

2



Select Cancel Bolus.

3



Select the bolus you wish to cancel.

NOTE

If only one bolus is being delivered, the meter skips Step 3. Proceed to Step 4.

4



Select OK. Bolus delivery is cancelled.

NOTE

Selecting Back returns you to the previous screen without cancelling the bolus.

6.6.2 Cancelling a Bolus from the Pump Menu

Main Menu > Pump > Bolus

1



From the Pump Menu, select Bolus.

2



Select Cancel Bolus.

3



Select the bolus you wish to cancel.

NOTE

If only one bolus is being delivered, the meter skips Step 3. Proceed to Step 4.

4



Select OK. Bolus delivery is cancelled.

NOTE

Selecting Back returns you to the previous screen without cancelling the bolus.

6.7 Delivering a Bolus Using Bolus Advice

With the meter and pump paired and bolus advice turned on, you have the ability to program and deliver boluses with the pump directly from the Bolus Advice menu on the meter.

The following conditions must be met before delivering a bolus using bolus advice:

- The meter must be paired with the pump.
- The pump must be in RUN mode.
- Bolus advice must be enabled on the meter.

NOTE

- When the meter is paired with the pump, bolus advice is calculated based on the insulin sensitivity defined in the meter settings.
- If you deliver a bolus directly on the pump without using the meter, the total bolus information is considered in future bolus advice. If this bolus is used for food intake, you can edit the bolus in your logbook to assign the portion of the bolus that was used for carbohydrate correction. This ensures that future bolus advice recommendations are calculated using the most complete information.
- Be patient when waiting for bolus advice results; the meter is processing numerous inputs.
- The confirmation steps are important for you to review the accuracy of the information you entered for bolus advice.
- For more information on bolus advice, refer to the **Bolus Advice** chapter of the **Accu-Chek Aviva Insight Diabetes Manager User's Manual**.

1

Insert a test strip and perform a blood glucose test.

NOTE

For information on performing a blood glucose test and entering bolus information with the Bolus Input menu, refer to the **Delivering a Bolus Using Bolus Advice** section of the **Bolus Advice** chapter of the **Accu-Chek Aviva Insight Diabetes Manager User's Manual.**

2



Enter your information as you normally do. Select Bolus.

3



If multiple health events have been selected, this screen displays "--- %"; otherwise proceed to the next step. You must enter a summarised health event percentage, even if this percentage is zero. Select Save.

4



Make any desired adjustments to the correction bolus or carbohydrate portions of the bolus, or to the total bolus.

NOTE

- If a Carbohydrate Bolus is entered and no amount has been entered for carbohydrates (Carbs displays No Entry in Step 2), you should consider entering an amount for carbohydrates. Select Back to enter an amount. An amount is not required, but the more complete the data the more accurate any future bolus advice recommendations are when using bolus advice.
- If you adjust either the Correction Bolus or Carbohydrate Bolus first: The ability to edit the Total Bolus is disabled; however, the Total Bolus updates accordingly.
- If you adjust the Total Bolus first: The ability to edit the Correction Bolus and Carbohydrate Bolus is disabled.
  - If Total Bolus is increased: The Correction Bolus is increased accordingly.
  - If Total Bolus is decreased: The Carbohydrate Bolus is decreased accordingly; once the Carbohydrate Bolus becomes 0, then the Correction Bolus is decreased accordingly.

5



Select Bolus Type to change the selected bolus type, if necessary, and proceed to Step 6. Otherwise, skip to Step 7.

6



Select the desired bolus type (Standard, Extended or Multiwave). Select Save.

NOTE

Pen/Syringe boluses do not require pairing with the pump and must be delivered manually. For more information on delivering Pen/Syringe boluses, refer to your pen/syringe User's Manual.

7



Select Next.

8

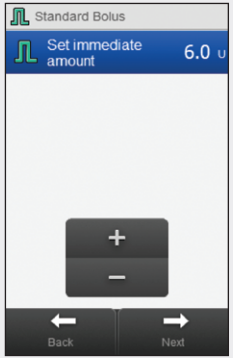

Select Next.

NOTE

When setting up a multiwave bolus, you can adjust the balance between the immediate amount and delayed amount, as long as the total amount of insulin delivered is equal to the units entered in previous steps. The immediate amount must also not fall below the recommended correction bolus from bolus advice.

9



Select OK to deliver the bolus.

NOTE

Selecting Back takes you back to the previous screen without delivering a bolus.

10



The pump delivers the bolus and the meter displays the Status screen showing the current bolus information.

NOTE

- If you selected the bolus type of **Manual On Pump** and the meter displays **Warning W-89** “A manual pump value has been set to zero,” the selected bolus amount was not delivered within 15 minutes and the logbook record is changed to zero units of insulin delivered. Review recent logbook data for accuracy, and edit if necessary.
- If you delivered the selected **Manual On Pump** bolus amount after more than 15 minutes have elapsed **or** if you delivered a different **Manual On Pump** bolus amount, the meter creates a new logbook record the next time the meter and pump communicate. The new record does not include the previous bolus advice information (e.g., health events or amount of carbohydrates). It is recommended that you edit the new record to include this information because it may impact future bolus advice recommendations.

7 Temporary Basal Rates

7.1 Programming a Basic Temporary Basal Rate (TBR)

Main Menu > Pump > Basal > Temporary Basal Rate > Basic TBR

1

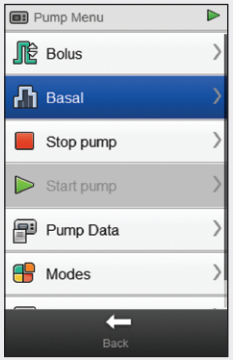

From the Pump Menu, select Basal.

2



Select Temporary Basal Rate.

3



Select Basic TBR.

4



Set the percentage and duration of the basic TBR. Select Next.

5



Select OK.

6



The meter displays the Status screen with the current TBR information.

7.2 Programming or Editing a Customised TBR

Main Menu > Pump > Basal > Temporary Basal Rate > Customized TBR

1



From the Pump Menu, select Basal.

2



Select Temporary Basal Rate.

3



Select ⊕ New TBR or select the existing customised TBR you wish to edit.

NOTE

Customised TBRs that you have previously programmed appear on this screen.

4



Set the percentage and duration of the customised TBR.

5



Select Edit Name.

6

Type the name you wish to use for the customised TBR. Select ✓.

7



To save your settings for the customised TBR without starting it, select Save. Otherwise, select Next.

8



Select OK.

9



The meter displays the Status screen with the current TBR information.

7.3 Cancelling an Active TBR

Main Menu > Pump > Basal > Temporary Basal Rate

1



From the Pump Menu, select Basal.

2



Select Temporary Basal Rate.

3



Select Cancel TBR.

4



Select OK. The active TBR is cancelled.

7.4 Deleting a Customised TBR

Main Menu > Pump > Basal > Temporary Basal Rate

1



From the Pump Menu, select Basal.

2



Select Temporary Basal Rate.

3



Select ✕ next to the name of the TBR you wish to delete.

4



Select OK. The TBR is deleted.

7.5 Additional TBR Function Information

The pump notifies you when a TBR has completed. You can disable this notification if desired.

If a TBR is not currently active, the TBR percentage is set to 100 %.

When a TBR is active, it remains in effect even if the basal profile is changed.

A TBR can only be programmed when the pump is in RUN mode.

When a TBR is active, the pump beeps and vibrates every hour.

Placing the pump in STOP mode cancels TBR delivery as well as any boluses being delivered.

For more information about pump messages, warnings and errors, and programming a TBR, see the **Accu-Chek Insight Insulin Pump User's Manual**.

8 Basal Profiles

8.1 Programming a Basal Profile

Main Menu > Pump > Basal > Program Basal Profile

1

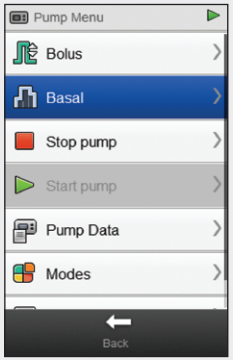

From the Pump Menu, select Basal.

2



Select Program Basal Profile.

3



Select the basal profile you wish to program.

4

Select Edit Name.

5

Type the name you wish to use for the basal profile. Select ✓.

6

Select a time block you wish to edit.

7



Set the End time and basal rate Amount. Select Save. Repeat this step for each time block you wish to edit.

NOTE

- You are only able to edit the end time of basal rate time blocks. The start time for each time block is the same as the end time for the previous time block.
- Basal rate time blocks are not identical to or shared with the time blocks for bolus advice.
- To add a new time block, set the end time of the last time block to the desired start time for the new time block.
- To delete a time block, set the end time of the time block equal to the start time of the time block.

8



Select Save.

9



Select OK. The meter saves the changes to the basal profile.

NOTE

- Selecting OK to save changes does **not** activate the basal profile.
- Selecting Back at any time takes you back to the Basal Profile Time Blocks screen where you can continue to adjust the settings of the selected basal profile.
- For more information on basal rates, refer to the **Accu-Chek Insight Insulin Pump User's Manual**.

8.2 Activating a Basal Profile

Main Menu > Pump > Basal > Activate Basal Profile

1



From the Pump Menu, select Basal.

2



Select Activate Basal Profile.

3



Select the basal profile you wish to activate.

4



If necessary, scroll the screen to review all the time blocks of the basal profile. Select ▶ Activate.

5



Select OK. The selected basal profile is active immediately.

NOTE

Selecting Back cancels the activation of the selected basal profile and takes you to the previous screen. The previously active basal profile remains active.

8.3 Clearing a Basal Profile

Main Menu > Pump > Basal > Program Basal Profile

1



From the Pump Menu, select Basal.

2



Select Program Basal Profile.

3



Select ⌀ next to the basal profile you wish to clear.

4



Select OK. The meter clears all saved settings for the selected basal profile and takes you back to the Program Basal Profile screen.

NOTE

Selecting Back at any time takes you back to the Program Basal Profile screen without clearing the selected basal profile.

9 Using Modes

9.1 Changing the Signal Mode of the Pump

Main Menu > Pump > Modes > Signal Mode

1

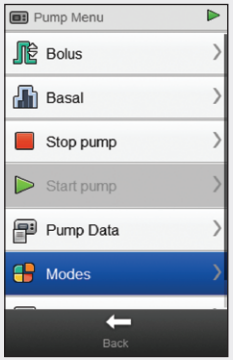

From the Pump Menu, select Modes.

2



Select Signal Mode.

3

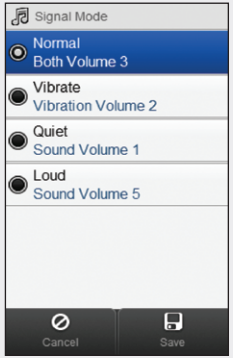

Press the radio button on the left side of the screen to activate a mode.

Press a mode's name to change its settings.

NOTE

For more information on the different signal modes on the pump, refer to the **Accu-Chek Insight Insulin Pump User's Manual**.

9.2 Turning On Flight Mode

Main Menu > Flight Mode

1



From the Main Menu, select Flight Mode.

2



Select Flight Mode on.

3

Select OK. Communication on both the meter and pump is disabled. Confirm that the ✈ symbol appears on the pump.

NOTE

You cannot turn flight mode back off on the pump by using the meter. Refer to the **Accu-Chek Insight Insulin Pump User's Manual** for instructions on turning off flight mode on the pump.

9.3 Turning Off Flight Mode

Main Menu > Flight Mode

1



From the Main Menu, select Flight Mode.

2



Select Flight Mode off.

3



Select OK.

NOTE

Refer to the **Accu-Chek Insight Insulin Pump User's Manual** for instructions on turning off flight mode on the pump.

10 Pump Settings

You can change many of the settings on the pump with the meter. They are the same settings that are viewed from the Settings menu on the pump. These settings are:

- Reminders
- Device Settings
- Therapy Settings
- Date and Time

These settings are stored on the pump and remain in effect even if the meter and pump are disconnected or the meter is turned off.

For detailed explanations of pump reminders, device settings and therapy settings, refer to the **Accu-Chek Insight Insulin Pump User's Manual**.

10.1 Pump Reminders

You can set pump reminders using the meter. There are four types of pump reminders:

- Deliver Bolus
- Missed Bolus
- Alarm Clock
- Infusion Set Change

The Deliver Bolus, Missed Bolus and Alarm Clock reminder types each contain up to five reminders. The Infusion Set Change reminder type contains only one reminder to change the infusion set of the pump at the set time.

NOTE

- Reminders are stored on the pump and occur on the pump even if the meter and pump are disconnected.
- Reminders do not automatically turn the meter on and display the reminder. The pump alerts you of a reminder. Turn on the meter or the pump to view the reminder and silence the alert.
- When a pump reminder displays on the meter, press **Mute** to silence the reminder for 60 seconds. Press **Dismiss** to dismiss the reminder permanently.

10.1.1 Setting Pump Reminders

Main Menu > Pump > Settings > Reminders

1



From the Pump Menu, scroll the screen and select Settings.

2



Select Reminders.

3



Select the type of reminder that you wish to set.

4



Select a reminder.

5



Select On to turn the reminder on.

6



Select Time.

7

Set the time. Select Save.

8



Select Tone.

9



Choose the tone to use for the reminder. Select Save.

NOTE

You can listen to a reminder tone by selecting ♫ next to it.

10



Select Status.

11



Choose the desired status.
Select Save.

Option	Description
Once	The pump plays the reminder tone starting at the chosen time until the reminder is muted, in which case the pump plays the reminder tone again in 60 seconds, or dismissed, in which case the reminder tone does not play again unless you turn on the reminder again from the Pump Reminders menu.
Repeat	The pump plays the reminder tone starting at the chosen time until the reminder is muted, in which case the pump plays the reminder tone again in 60 seconds, or dismissed, in which case the pump repeats the reminder every day at the chosen time until the reminder is turned off from the Pump Reminders menu.

12



Select Edit Name.

13

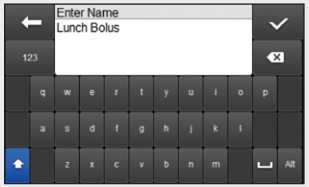

Type the name you wish to use for the reminder.
Select ✓.

14



Select Save.

10.1.2 Setting the Infusion Set Change Reminder

Main Menu > Pump > Settings > Reminders > Infusion Set Change

1



From the Pump Menu, select Settings.

2



Select Reminders.

3



Select Infusion Set Change.

4



Select On to turn the Infusion Set Change reminder on.

5



Select Remind In (days).

6

Set the number of days when the reminder will occur. Select Save.

NOTE

The reminder can be set for 1 day, 2 days or 3 days.

7



Select Set Time.

8

Set the time of day when the reminder will occur. Select Save.

9



Select Set Tone.

10



Choose the tone to use for the reminder. Select Save.

NOTE

You can listen to a reminder tone by selecting ♫ next to it.

11



Select Status.

12



Choose the desired status. Select Save.

13



Select Save.

10.2 Therapy Settings

You can change the pump therapy settings from the meter. These settings are:

- Automatic Off
- Bolus
- Infusion Set
- Cartridge Warning Level

⚠ WARNING

It is vital that you use the correct therapy settings. Otherwise, you might get a wrong amount of insulin with the risk of hypo- or hyperglycaemia. The therapy setting should be provided by your healthcare professionals and you should discuss with them before making any changes.

10.2.1 Setting the Automatic Off Timer

Main Menu > Pump > Settings > Therapy Settings > Automatic Off

Automatic Off is a safety feature that stops insulin delivery and triggers a Maintenance message if no pump keys are pressed and no commands are sent to the pump from the meter within a set amount of time. For more information about the Automatic Off feature, refer to the **Accu-Chek Insight Insulin Pump User's Manual**.

1



From the Pump Menu, select Settings.

2



Select Therapy Settings.

3

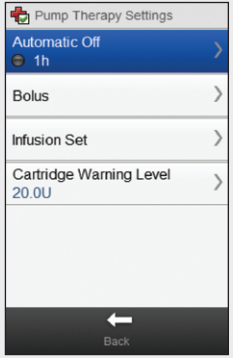

Select Automatic Off.

4

Select On to turn the Automatic Off timer on.

5

Set the time. Select Save.

10.2.2 Bolus Settings

You can change the bolus settings on the pump using the meter. These settings are:

- Quick Bolus Increment
- Delivery Speed
- Maximum Bolus Amount
- Lag Setting

Refer to the **Setting the Quick Bolus Increment**, **Setting the Delivery Speed**, **Setting the Maximum Bolus Amount** and **Changing the Lag Setting** sections for instructions for changing the bolus settings.

Main Menu > Pump > Settings > Therapy Settings > Bolus

1



From the Pump Menu, select Settings.

2



Select Therapy Settings.

3



Select Bolus.

Setting the Quick Bolus Increment

Main Menu > Pump > Settings > Therapy Settings > Bolus > Quick Bolus Increment

NOTE

The Quick Bolus Increment setting changes how much insulin is added by each press of the pump keys to the total amount of a Quick Bolus.

1



From the Bolus Settings menu, select Quick Bolus Increment.

WARNING

Make sure that you know and use the correct bolus increment. Using the incorrect bolus increment will deliver the wrong insulin dose.

2



Choose the appropriate quick bolus increment. Select Save.

Setting the Delivery Speed

Main Menu > Pump > Settings > Therapy Settings > Bolus > Delivery Speed

1



From the Bolus Settings menu, select Delivery Speed.

2



Choose the appropriate delivery speed. Select Save.

Setting the Maximum Bolus Amount

Main Menu > Pump > Settings > Therapy Settings > Bolus > Max Bolus Amount

1



From the Bolus Settings menu, select Max Bolus Amount.

2



Set the maximum amount. Select Save.

Changing the Lag Setting

Main Menu > Pump > Settings > Therapy Settings > Bolus > Lag Setting

1



From the Bolus Settings menu, select Lag Setting.

2



Select On or Off as appropriate. Select Save.

NOTE

With lag time turned on, you can set the lag time each time you program a new bolus.



When programming the bolus amount (for Standard bolus) or the bolus amount and delayed duration (Extended or Multiwave bolus), Set lag time also appears.

Adjust the default lag time using Set lag time.

Select Next.

10.2.3 Changing the Infusion Set Settings

Main Menu > Pump > Settings > Therapy Settings > Infusion Set

1



From the Pump Menu, select Settings.

2



Select Therapy Settings.

3



Select Infusion Set.

4

Set the tubing fill amount and the cannula fill amount. Select Save.

10.2.4 Setting the Cartridge Warning Level

Main Menu > Pump > Settings > Therapy Settings > Cartridge Warning Level

1



From the Pump Menu, select Settings.

2



Select Therapy Settings.

3



Select Cartridge Warning Level.

4



Set the warning amount.
Select Save.

10.3 Device Settings

You can change the pump device settings from the meter. These settings are:

- Mode Settings
- Key Lock
- Language

10.3.1 Pump Signal Modes: Sound and Vibration

You can use the meter to choose whether you want the pump to sound, vibrate or do both at the same time as an event (for example, a reminder) occurs. You can adjust the sound volume.

Main Menu > Pump > Settings > Device Settings > Mode Settings

1



From the Pump Menu, select Settings.

2



Select Device Settings.

3



Select Mode Settings.

4

Choose a mode.

5



Choose the desired mode setting. Set the volume. Select Save.

6



Repeat Steps 4 and 5 to change the settings for additional modes as desired. Select Back when finished.

10.3.2 Pump Signal Modes: Signal Suspension

You can suspend the signals for Warnings for a specified period of time. However, since Error and Maintenance messages require your immediate attention, you cannot suspend these event signals. Also, the Reminders you programmed will not be suspended.

A signal suspension can be set to occur once, or it can be set to repeat at the same time every day.

Main Menu > Pump > Settings > Device Settings > Mode Settings > Signal Suspension

1



From the Pump Menu, select Settings.

2



Select Device Settings.

NOTE

Any Warnings that occur during the signal suspension period appear when the meter turns on.

3

Select Mode Settings.

4



Select Signal Suspension.

5

Select On or Off. Set the Start time and End time. Scroll the screen and choose either Once or Repeat. Select Save.

6



Select Back.

10.3.3 Setting the Key Lock Time

Main Menu > Pump > Settings > Device Settings > Key Lock

1



From the Pump Menu, select Settings.

2



Select Device Settings.

3



Select Key Lock.

4

Set the key lock time. Select Save.

NOTE

- The pump keys automatically lock if they are not used within the amount of time set using the key lock setting.
- The key lock only affects the manual operation of the pump, even when the key lock time is set using the meter.

10.3.4 Setting the Pump Language

Main Menu > Pump > Settings > Device Settings > Language

1



From the Pump Menu, select Settings.

2



Select Device Settings.

3



Select Language.

4

Choose the desired language.
Select Save.

10.4 Setting the Pump Date and Time

You can set the pump date and time using the meter.

NOTE

It is very important to set the correct date and time. Otherwise you may not receive the correct amount of insulin at the correct time.

When the meter is paired with the pump, changing the date and time on the meter automatically changes the date and time on the pump.

After you change the date or time, the meter displays the notification that the date and time has been updated on both meter and pump. Select OK.

Main Menu > Pump > Settings > Date and Time

1



From the Pump Menu, select Settings.

2



Select Date and Time.

3

Select the desired time format (12 hr or 24 hr).

4



Set the date and time. Select Save.

11 My Data

11.1 Overview

Analysing your information stored in the meter is an effective way for you and your healthcare professional to determine how well you are controlling your diabetes. This analysis is a valuable tool for making improvements to your diabetes management. The reports the meter displays help you get the most from your Accu-Chek Aviva Insight diabetes manager.

The meter generates graphs and reports to help you analyse the information stored in the meter. Graphs can be a good way to view your blood glucose results. The meter can display a line graph to depict the trends of your blood glucose results with other information, such as your bolus history, a graph showing result ranges for a standard day or a standard week, and a pie chart with different colours to illustrate the number of test results within, above or below your blood glucose target range.

NOTE

- Reviewing reports consumes battery power. It is advisable to connect the meter to the charger while reviewing reports.
- Blood glucose is sometimes shortened to bG, but it means the same thing.

11.2 The Logbook

From the logbook records stored in the meter, you are able to view a specific blood glucose result with its attributes (e.g., meal time, carbohydrates, health event and bolus). In addition, for a specific logbook record, you are able to change or add to its attributes.

NOTE

- The logbook on the meter replaces the physical blood glucose diary you may have kept in the past.
- Logbook data cannot be changed if that data was used to calculate bolus advice.

The meter automatically stores up to 2,000 logbook records with the time and date. You can review up to the last 250 logbook records on the meter or up to 2,000 logbook records using a computer with compatible software. Logbook records are stored from the newest to the oldest.

Each logbook record can contain:

- Date and time
- Blood glucose result
- Meal time (events)
- Carbohydrate intake
- Health event
- Bolus type
- Bolus amount
- Note
- Quick Notes

NOTE

- **Do not change your therapy based on one individual record or test result in the logbook.**
- This chapter shows sample screens. The screens may look slightly different from the screens on the meter. If you have any questions about the meter screens, contact Roche.
- The information in the logbook is saved when you replace the meter battery. You should check the time and date after replacing the battery. For more information on changing the battery, see the **Care and Maintenance** chapter of the **Accu-Chek Aviva Insight Diabetes Manager User's Manual**.
- It is very important to have the correct time and date set. Having the correct time and date setting helps ensure accurate interpretation of information by you and your healthcare professional.
- Once 2,000 records are in the logbook, adding a new record causes the oldest logbook record to be deleted.
- Control results are stored in the meter, but cannot be reviewed in the logbook. Control results can be reviewed using a computer with compatible software.
- Before reviewing logbook records or control results on a PC, the stored logbook records must first be transferred to a PC running a compatible software application. For product availability, contact Roche.
- Control results are not used in any report or graph on the meter.



11.2.1 Understanding the Logbook

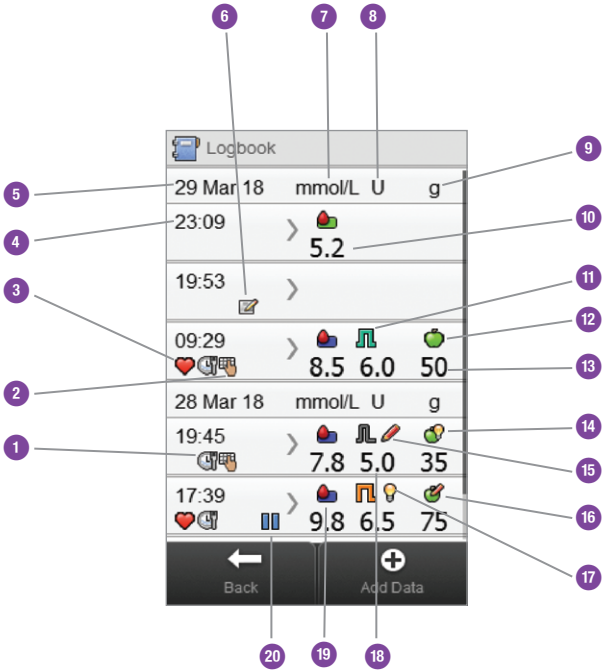

1	Meal time icon
2	Note icon
3	Health event icon
4	Time of record
5	Date of record
6	Quick Notes icon
7	Indicates bG column
8	Indicates bolus column
9	Indicates carbohydrate column
10	Blood glucose result

11	Bolus type icon
12	Carbohydrates icon
13	Carbohydrate amount
14	Carbohydrates advice accepted icon
15	Bolus advice not accepted icon
16	Carbohydrates advice not accepted icon
17	Bolus advice accepted icon
18	Bolus amount
19	bG value range icon
20	Pump paused icon

NOTE

The Logbook screen displays the records in the order in which they occurred with the most recent record shown on top.

Icon descriptions

Icon	Icon name	Description
	bG Value Range Indicator	Icon background colour indicates where the blood glucose result falls within the target range. The background colours of this icon represent: ▸ Green: within target range ▸ Yellow: below target range ▸ Red: hypo ▸ Blue: above target range or hyper
	Meal time	Icon is displayed when information exists for this record regarding meal time.
	Carbohydrates	Icon is displayed when information exists for this record regarding carbohydrates.
	Carbohydrates advice accepted	Icon is displayed when the carbohydrate amount from the bolus advice recommendation hypo warning screen was used.

Icon	Icon name	Description
	Carbohydrates advice not accepted	Icon is displayed when the carbohydrate amount from the bolus advice recommendation hypo warning screen was changed.
	Health event	Icon is displayed when information exists for this record regarding health events.
	Standard bolus not confirmed	Delivery has not been confirmed by the pump.
	Standard bolus confirmed	Delivery has been confirmed by the pump.
	Extended bolus not confirmed	Delivery has not been confirmed by the pump.
	Extended bolus confirmed	Delivery has been confirmed by the pump.
	Multiwave bolus not confirmed	Delivery has not been confirmed by the pump.
	Multiwave bolus confirmed	Delivery has been confirmed by the pump.

Icon	Icon name	Description
	Bolus advice accepted	Bolus advice from the meter was accepted.
	Bolus advice not accepted	Bolus advice from the meter was changed prior to delivery.
	Manual on pump	Delivery has not been confirmed by the pump.
	Bolus manually delivered using pen/syringe	Bolus delivered using pen/syringe. Bolus was not delivered by the pump.
	Pump paused	Pump was paused during a bolus and then resumed to complete bolus delivery.
	Quick Notes	Icon is displayed when information exists for this record regarding Quick Notes.
	Notes	Icon is displayed when information exists for this record regarding a note.

11.2.2 Viewing and Adjusting Logbook Data

Main Menu > My Data > Logbook

NOTE

- Logbook data that has been used for bolus advice (with the exception of notes) cannot be adjusted.
- Blood glucose results cannot be adjusted.
- Once you begin delivering a bolus using the pump, any changes you make to the logbook record in My Data on the meter do not modify the bolus that is being delivered by the pump.

1



From the Main Menu, select My Data.

2



Select Logbook.

3



Select the desired logbook record. For a logbook record with Quick Notes only, go to Step 5.

NOTE

- Scroll down to view additional records if they are present.
- Logbook records which have been used for bolus advice contain either the Bolus advice accepted icon: or the Bolus advice not accepted icon: . These records are locked and can be viewed but not adjusted.
- Locked logbook records do not display the Save button at the bottom of the individual data item screens. Only the Back button is displayed.

4



To view and adjust an entry, select it and refer to the instructions on the following pages. When you have finished, select Back to return to the My Data menu.

Screens for Viewing and Adjusting Entries in the Logbook

Meal Time



Choose applicable meal time. Select Save.

Carbohydrates

Set the amount of carbohydrates consumed. Select Save.

Health Events





Choose up to four health events. Select Save.

If bolus advice is turned on, and multiple health events have been selected, this screen displays “--- %”. You must enter a summarised health event percentage for the selected health events, even if this percentage is zero. Select Save.

Bolus

Set bolus amounts. Select Save.

NOTE

If a Carbohydrate Bolus is entered and no Carbohydrate Amount has been entered for carbohydrates (Carbohydrates displays No Entry on the bG Record screen in Step 4), you are prompted to enter an amount for carbohydrates. An amount is not required, but the more complete the data the more accurate any future bolus advice recommendations are when using bolus advice.

Note

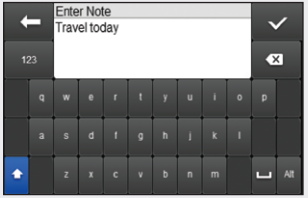

Type a note to save with this record. Select ✓.

5



Select Quick Notes to make an update. Select Note to type a note using the keyboard. Select Back to return to Step 3.

11.2.3 Adding New Data to the Logbook

Main Menu > My Data > Add Data

1



From the Main Menu, select My Data.

2



Select ⊕ Add Data.

3



Select any of the options on the Add Data screen and refer to the instructions on the following pages.

When you have finished, select Save to save your entry and return to the My Data menu.

Screens for Adding New Data

Date and Time



Set the date and time. Select Save.

Meal Time



Choose an applicable meal time. Select Save.

Carbohydrates



Set the amount of carbohydrates consumed. Select Save.

Health Events



Choose up to four health events. Select Save.



If bolus advice is turned on, and multiple health events have been selected, this screen displays “--- %”. You must enter a summarised health event percentage for the selected health events, even if this percentage is zero. Select Save.

Bolus

Set bolus amounts. Select Save.

NOTE

If a Carbohydrate Bolus is entered and no amount has been entered for carbohydrates (Carbs displays No Entry in Step 3), you are prompted to enter an amount for carbohydrates. An amount is not required, but the more complete the data the more accurate any future bolus advice recommendations are when using bolus advice.

Note

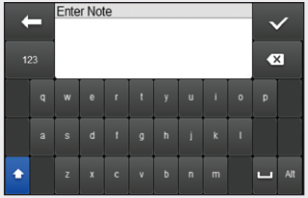

Type a note to save with this record. Select ✓.

11.3 The Trend Graph

With the trend graph, the meter displays your blood glucose trends and other information using logbook data for the time scale and meal time you choose.

11.3.1 Understanding the Trend Graph

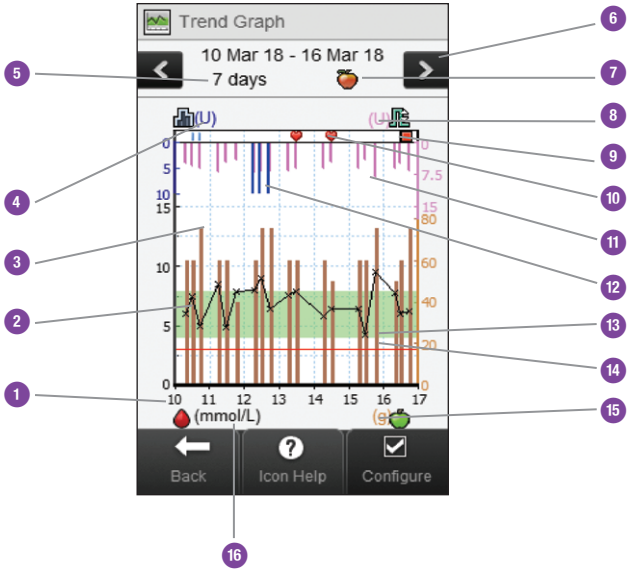

1	**Times of day or days of the month**	
2	**Blood glucose result**	Displayed as Xs and connected with lines
3	**Carbohydrate value**	Brown bar: height shown is in relation to the carbohydrate amount
4	**Basal unit of measurement**	
5	**Time scale**	

6	**Scroll left/right buttons**	Moves forward or back in time by the time scale chosen. Example: For a 7-day time scale, selecting the scroll left icon shows the data from the 7 days before the dates currently shown.
7	**Selected meal time**	
8	**Bolus unit of measurement**	
9	**Pump stopped icon**	Indicates pump was stopped
10	**Health Event**	Indicates a Health Event exists for the record
11	**Bolus**	Pink bar: height shown is in relation to the bolus insulin amount

12	**Basal value**	Blue line: indicates the basal insulin amount
13	**Green area**	Indicates blood glucose target range
14	**Hypo warning limit**	Red horizontal line
15	**Carbohydrate unit of measurement**	
16	**Blood glucose unit of measurement**	
17	**Arrow**	(Not shown) Indicates blood glucose data extends beyond screen
18	**Pump paused icon**	(Not shown) Indicates when the pump was paused during insulin delivery

NOTE

- If data is not available, the No Data Available screen is displayed.
- Trend graphs do not include corrupt results or control results
- On the upper right side of the graph, the maximum bolus amount indicator is the pink tick mark with the largest value shown beside it (on this example screen: 15 U). The purpose of this indicator is to adjust the scale for the top portion of the graph based on the single biggest bolus insulin amount (callout 11) delivered for the time chosen (callout 5). The maximum bolus amount indicator values available on the meter are 1, 5, 15, 30 and 60 U. For example, if the single biggest bolus insulin amount is 8 U, then the meter scales the upper graph to be between 0 and 15 U.

NOTE

- On the lower right side of the graph, the maximum carbohydrate amount indicator is the brown tick mark with the largest value shown beside it (on this example screen: 80 g). The purpose of this indicator is to adjust the scale for the bottom portion of the graph based on the single biggest carbohydrate amount (callout 3) for the time chosen (callout 5). The maximum carbohydrate amount indicator values available on the meter are 40, 80, 120, 160, 200 and 240 g, or the equivalent scale for BE, KE or CC. For example, if the single biggest carbohydrate amount is 76 g, then the meter scales the lower graph to be between 0 and 80 g.
- On the upper left side of the graph, the maximum basal amount indicator is the blue tick mark with the largest value shown beside it (on this example screen: 10 U). The purpose of this indicator is to adjust the scale for the top portion of the graph based on the single biggest basal insulin amount (callout 12) delivered for the time chosen (callout 5). The maximum basal amount indicator values available on the meter are 1, 2, 5, 10, 20 and 40 U. For example, if the single biggest basal insulin amount is 9 U, then the meter scales the upper graph to be between 0 and 10 U.

11.3.2 Viewing the Trend Graph

Main Menu > My Data > Trend

1



From the Main Menu, select My Data.

2



Select Trend.

3



Select Configure to change how the trend graph displays your trend data.

NOTE

Select ? to view a list of trend icons and their explanations.

4



Select any of the options on the Configure Graph screen and refer to the instructions in the rest of this section. When you have finished, select Back to return to the trend graph displaying your data in the manner you selected.

Screens for Configuring the Trend Graph

Time Scale



Select the time scale. Select Save.

Data Options



Select 1 or more data options. Select Save.

Meal Time

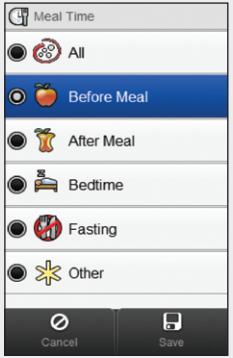

Select the meal time. Select Save.

11.4 The Standard Week

With the Standard Week graph, the meter displays your blood glucose averages, number of tests and standard deviations for each day of an average week, calculated using logbook data from the time scale and meal time you choose.

NOTE

The standard deviation measures how spread out the blood glucose results are from the blood glucose average. A high standard deviation means the blood glucose results vary greatly around the blood glucose average.

11.4.1 Understanding the Standard Week Graph and Table

Standard Week Graph

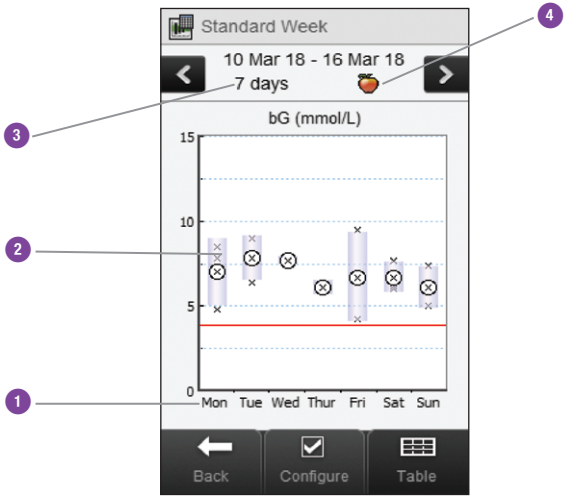

1	**Days of week**	
2	**Box for each day**	▶ The top of the box indicates the standard deviation above the average and the bottom of the box indicates the standard deviation below the average. The box is not displayed if there is not enough data to determine standard deviation. ▶ The top of the box is open if the standard deviation is off the top of the graph. ▶ Box and “X” are not displayed for a day if no data is found.
3	**Time scale**	
4	**Meal time selection**	

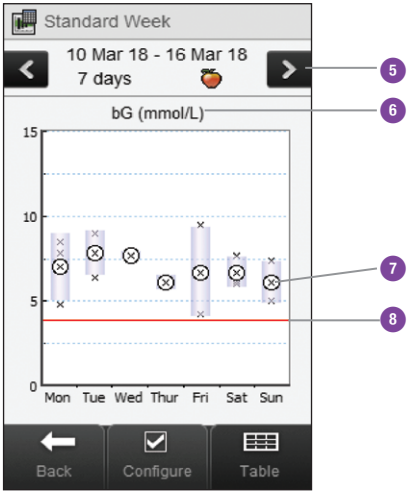

5	**Scroll left/right buttons**	Moves forward or back in time by the time scale chosen. Example: For a 7-day time scale, selecting the scroll left icon shows the data from the 7 days before the dates currently shown.
6	**Blood glucose unit of measurement**	
7	**X**	Indicates each blood glucose result. “X” in the centre of a circle indicates the average of all blood glucose results for the selected criteria.
8	**Hypo warning limit**	Red horizontal line
9	**Arrow**	(Not shown) Indicates that there is data off the top of the graph.

Standard Week Table

Select Table to switch to the standard week table. The standard week table displays the same data as the standard week graph in table format. To return to the standard week graph from the standard week table, select Graph.

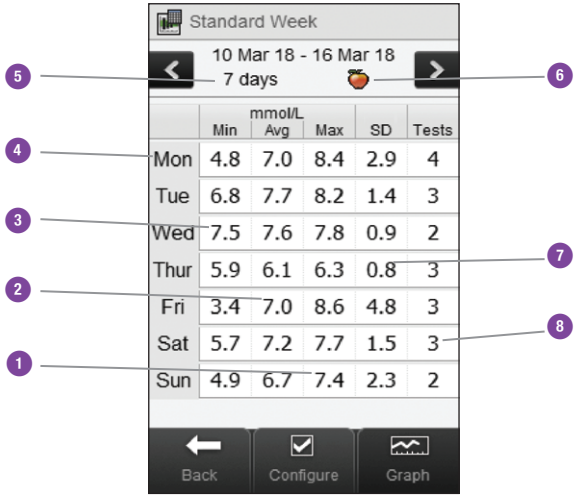

1	Highest blood glucose result for each day of the week
2	Blood glucose average for each day of the week
3	Lowest blood glucose result for each day of the week
4	Day of week
5	Time scale
6	Meal time selection
7	Standard deviation (SD) for each day of the week
8	Number of tests for each day of the week

11.4.2 Viewing Standard Week Data

Main Menu > My Data > Standard Week

1



From the Main Menu, select My Data.

2



Select Standard Week.

NOTE

- If there is no data available to display the standard week graph and table for the time scale or meal time chosen, the No Data Available screen is displayed.
- The standard week graph and table do not include corrupt results, control results, HI values or LO values.

3



To change the time scale and meal time displayed for the standard week, select Configure.

4



Select either of the options on the Configure Data screen and refer to the instructions in the rest of this section. Select Back when finished to return to the Standard Week graph or table.

Screens for Configuring Standard Week Data

Time Scale



Select a time scale. Select Save.

Meal Time



Select a meal time. Select Save.

11.5 The Standard Day

With the Standard Day graph, the meter displays your blood glucose averages, number of tests and standard deviations for each time block, calculated using logbook data from the time scale and meal time you choose.

NOTE

Refer to the **Changing Meter Settings** chapter of the **Accu-Chek Aviva Insight Diabetes Manager User's Manual** for instructions on setting up the time blocks.

NOTE

The standard deviation measures how spread out the blood glucose results are from the blood glucose average. A high standard deviation means the blood glucose results vary greatly around the blood glucose average.

11.5.1 Understanding the Standard Day Graph and Table

Standard Day Graph

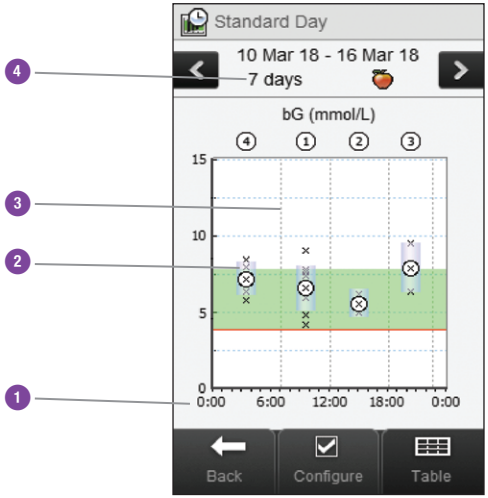

1	**Time of day**	
2	**Box for each time block**	▶ The top of the box indicates 1 standard deviation above the average and the bottom of the box indicates 1 standard deviation below the average. The box is not displayed if there is not enough data to determine standard deviation. ▶ The top of the box is open if the standard deviation is off the top of the graph. ▶ Box and “X” are not displayed for a time block if no data is found.
3	**Time blocks**	Separated by the vertical dashed line
4	**Time scale**	

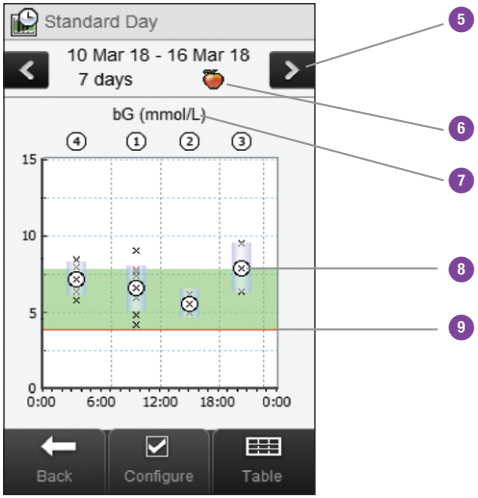

5	**Scroll left/right buttons**	Moves forward or back in time by the time scale chosen. Example: For a 7-day time scale, selecting the scroll left icon shows the data from the 7 days before the dates currently shown.
6	**Meal time selection**	
7	**Blood glucose unit of measurement**	
8	**X**	▸ Indicates each blood glucose result. ▸ “X” in the centre of a circle indicates the average of all blood glucose results for the selected criteria.
9	**Hypo warning limit**	Red horizontal line
10	**Arrow**	(Not shown) Indicates that there is data off the top of the graph.

Standard Day Table

Select Table to switch to the standard day table. The standard day table displays the same data as the standard day graph in table format. To return to the standard day graph from the standard day table, select Graph.

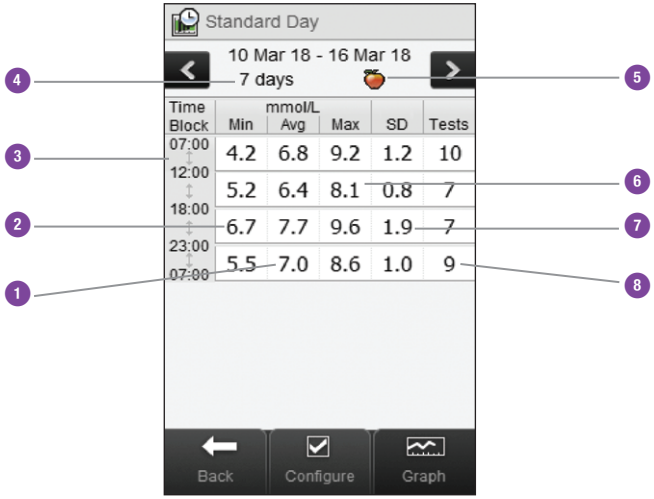

1	Blood glucose average for each time block
2	Lowest blood glucose result for each time block
3	Time block
4	Time scale
5	Meal time selection
6	Highest blood glucose result for each time block
7	Standard deviation (SD) for each time block
8	Number of tests for each time block

11.5.2 Viewing Standard Day Data

Main Menu > My Data > Standard Day

1



From the Main Menu, select My Data.

2



Select Standard Day.

NOTE

- If there is no data available to display the standard day graph and table for the time scale or meal time chosen, the No Data Available screen is displayed.
- The standard day graph and table do not include corrupt results, control results, HI values or LO values.

3



To change the time scale and meal time displayed, select Configure.

4



Select either of the options on the Configure Data screen and refer to the instructions in the rest of this section. Select Back when finished to save any changes and return to the standard day graph or table.

Screens for Configuring Standard Day Data

Time Scale



Select a time scale. Select Save.

Meal Time



Select a meal time. Select Save.

11.6 Target Data

The meter displays a pie chart and table illustrating your blood glucose results as “Above”, “Within”, “Below” and “Hypo” for the time scale and meal time you choose.

11.6.1 Understanding the Target Chart and Target Table

Target Chart

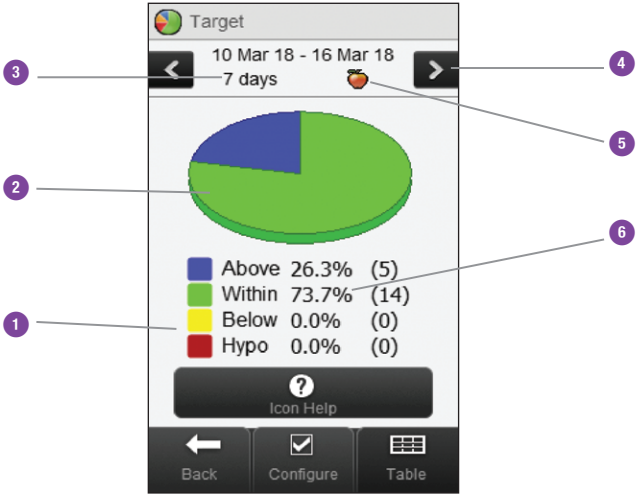

1	**Legend**	Blood glucose result categories
2	**Target chart**	Represents the percentages for the blood glucose result categories
3	**Time scale**	
4	**Scroll left/right buttons**	Moves forward or back in time by the time scale chosen. Example: For a 7-day time scale, selecting the scroll left icon shows the data from the 7 days before the dates currently shown.
5	**Meal time selection**	
6	**Percentage of occurrence**	(Number shown in parentheses represents the number of occurrences)

Target Table

Select Table to switch to the target table. The target table displays the same data as the target chart in table format.

To return to the target chart from the target table, select Chart.

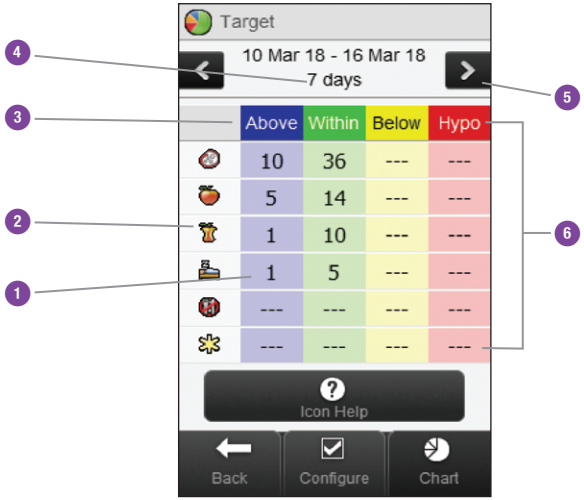

1	**Number of occurrences**	
2	**Meal time selection**	
3	**Legend**	Blood glucose result categories
4	**Time scale**	
5	**Scroll left/right buttons**	Moves forward or back in time by the time scale chosen. Example: For a 7-day time scale, selecting the scroll left icon shows the data from the 7 days before the dates currently shown.
6	**Target table**	

11.6.2 Viewing Target Data

Main Menu > My Data > Target

1



From the Main Menu, select My Data.

2



Select Target.

NOTE

- If there is no data available to display the target chart and table for the time scale or meal time chosen, the No Data Available screen is displayed.
- The target chart and table do not include corrupt results, control results, or HI and LO results.

3



To change the time scale and meal time displayed, select Configure.

4



Select either of the options on the Configure Data screen and refer to the instructions in the rest of this section. Select Back when finished to save any changes and return to the target chart or table.

Screens for Configuring Target Data

Time Scale



Select a time scale. Select Save.

Meal Time



Select a meal time. Select Save.

11.7 The bG Averages Table

The bG Averages table displays your blood glucose averages and standard deviations for the time scale and meal time you choose.

NOTE

The standard deviation measures how spread out the blood glucose results are from the blood glucose average. A high standard deviation means the blood glucose results vary greatly around the blood glucose average.

11.7.1 Understanding the bG Averages Table

bG Averages Table

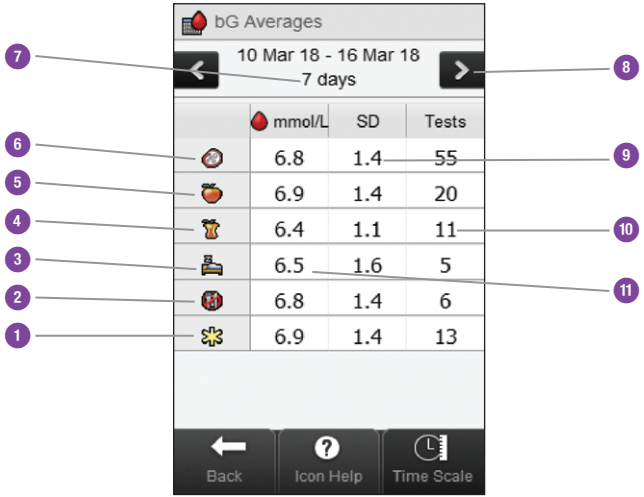

1	**Other icon**	Data for all test results marked as Other
2	**Fasting icon**	Data for all test results marked as Fasting
3	**Bedtime icon**	Data for all test results marked as Bedtime
4	**After meal icon**	Data for all test results marked as After meal
5	**Before meal icon**	Data for all test results marked as Before meal
6	**All icon**	Combined data from all meal times
7	**Time scale**	

8	**Scroll left/right buttons**	Moves forward or back in time by the time scale chosen. Example: For a 7-day time scale, selecting the scroll left icon will show the data from the 7 days before the dates currently shown.
9	**Blood glucose standard deviation**	Calculated for the meal time
10	**Number of tests**	Used to calculate the averages and standard deviation of each meal time
11	**Blood glucose average**	Calculated for the meal time

11.7.2 Viewing the bG Averages Table

Main Menu > My Data > bG Averages

1



From the Main Menu, select My Data.

2



Select bG Averages.

NOTE

- If there is no data available to display the bG averages table for the time scale or meal time chosen, the No Data Available screen is displayed.
- Calculations do not include corrupt results, control results, HI values or LO values.

3

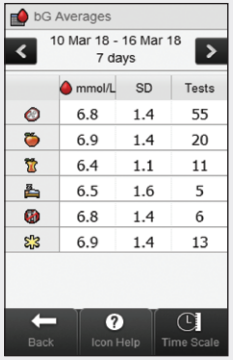

Select Time Scale to adjust the time scale of the bG Averages table.

NOTE

Select ⓘ to view a list of meal time icons and their explanations.

4



Choose a time scale. Select Save.

5



Select Back when finished to return to the My Data menu.

12 Technical Information

The RF channel utilised for communication is not an open channel. The meter can only communicate with the device it is paired with. Therefore, other Bluetooth wireless technology devices (cell phones, printers, etc.) cannot be paired with, communicate with, or access your personal information on the meter.

Declaration of Conformity

Roche hereby declares that the Accu-Chek Insight diabetes therapy system conforms with the basic requirements and other relevant regulations of the European Directive 2014/53/EU. The conformity declaration may be found at the following Internet address: http://declarations.accu-chek.com

Maximum Transmitted Power

Accu-Chek Aviva Insight meter: 30 mW

Compliance With IEC or ISO Standards

Additional equipment connected to medical electrical equipment must comply with the respective IEC or ISO standards (e.g., IEC 60950 or IEC 62368 for data processing equipment). Furthermore, all configurations must comply with the requirements for medical electrical systems (see Clause 16 of the latest valid version of IEC 60601-1). Anyone who connects additional equipment to medical electrical equipment configures a medical system and is therefore responsible for making sure that the system complies with the requirements for medical electrical systems. If in doubt, consult your local representative or the technical service department.

Standard/directive references:

- IEC 60601-1:2012: 7.9.2.3, 7.9.2.5, 8.1.a, 8.2.1, 14.13, 16, 16.1, 16.2.d
- MDD 93/42/EEC: Annex I clause 13.6.c

12.1 Explanation of Symbols

These symbols may appear on the packaging, on the type plate, and in the User's Manual for the meter.

	Consult instructions for use
	Caution, refer to safety-related notes in the instructions for use accompanying this product.
	Temperature limitation (store at)
	Manufacturer
REF	Catalogue number
IVD	In vitro diagnostic medical device
GTIN	Global Trade Item Number

CE 0088	This product fulfils the requirements of the European Directive 98/79/EC on in vitro diagnostic medical devices.
CE	This product fulfils the requirements of the European Directive 1999/5/EC on radio and telecommunications terminal equipment (R&TTE).
	Custom lithium-ion rechargeable battery
LOT	Batch code
SN	Serial number
	Use by
	Manufacturer date

12.2 List of Icons

The following table contains the icons and icon names which may appear on the meter display when the meter is paired with a pump. All of the other icons can be found in the **Technical Information** chapter of the **Accu-Chek Aviva Insight Diabetes Manager User's Manual**.

Icon Name	Icon
Activate	
Alarm Data	
Basal Profile (Activate)	
Basal Profile (Program)	
Battery (Pump)	
Bolus Data	

Icon Name	Icon
Cancel Bolus	
Cartridge (Pump)	
Daily Total	
Delayed Duration	
Extended Bolus	
Extended Bolus Paused	

Icon Name	Icon
Extended Bolus Unconfirmed	
Lag Time	
Multiwave Bolus	
Multiwave Bolus Delayed Amount	
Multiwave Bolus Immediate Amount	
Multiwave Bolus Paused	

Icon Name	Icon
Multiwave Bolus Unconfirmed	
Pump or Manual on Pump Bolus	
Pump Data	
Pump Mode	
Pump Paused	
Pump Running or Start Pump	

Icon Name	Icon
Pump Settings	
Pump Stopped or Stop Pump	
Pump Timer	
Standard Bolus or Bolus	
Standard Bolus Paused	
Standard Bolus Unconfirmed	

Icon Name	Icon
Temporary Basal Rate	
Temporary Basal Rate Data	
Therapy settings	
Version	
Video	

13 Troubleshooting

This chapter specifically addresses the issues that may occur with the pairing of the meter and pump. For general troubleshooting information, refer to the **Troubleshooting** chapter of the **Accu-Chek Aviva Insight Diabetes Manager User's Manual**. For troubleshooting pump messages that appear on the meter, refer to the **Accu-Chek Insight Insulin Pump User's Manual**.

NOTE

If you have a problem with the pairing of the meter and pump that is not addressed in this chapter, contact Roche.

Problem	Possible Cause	Possible Solution
No devices found information message	No Bluetooth-activated device is within range of the meter.	▶ Ensure that the pump and meter are no further than 2 metres apart. ▶ Select OK to return to the Set Up New Pairing menu. Place the pump in Add Device mode and try the pairing again.
Paired pump information message	The meter is already paired with a pump.	Select OK to return to the Communication menu and refer to the **Unpairing the Meter and Pump** section of the **Meter and Pump Communication** chapter of this User's Manual to remove the current pairing.
Device not paired screen appears with the message The meter was not able to pair with [pump name].	▶ The pump battery has died. ▶ The pump and meter are out of communication range. ▶ There is an obstruction between the pump and meter.	▶ Change the pump battery. ▶ Ensure that the pump and meter are no further than 2 metres apart. ▶ Ensure there are no obstructions between the pump and the meter.

Problem	Possible Cause	Possible Solution
Device not paired screen appears with the message [Pump name] is already paired to a meter. Unpair the pump from the meter first.	▶ The pump is already paired with another meter.	▶ Remove the current pairing from the pump. Refer to the **Accu-Chek Insight Insulin Pump User's Manual** for instructions on unpairing the meter and pump.
	▶ The pump and meter are already paired to each other.	▶ No further action is needed.
Maximum paired devices information message	The meter is paired with the maximum number of devices.	Select OK to return to the Communication menu, select Manage Current Pairings, and remove one of the currently paired devices.
Connection lost M-68 maintenance message	▶ The pump battery has died. ▶ The pump and meter are out of communication range. ▶ A pump key has been pressed, temporarily disabling communication between the meter and pump.	▶ Change the pump battery. ▶ Ensure that the meter and pump are no further than 2 metres apart. ▶ Wait for the pump display to timeout and the meter and pump to automatically resume communication.

Problem	Possible Cause	Possible Solution
Communication lost M-27 maintenance message	The meter and pump have timed out while waiting for pairing confirmation.	Repeat the steps from the **Pairing the Meter and Pump** section of this User's Manual and follow the on-screen instructions on both devices.
Pump not able to complete task M-83 maintenance message	Communication has been lost between the meter and pump.	When this message is displayed during an attempted bolus insulin delivery by the pump, perform the following: 1. Press "OK" on the M-83 message to confirm it. 2. Power down the meter. 3. Check the pump to determine the amount of insulin that was actually delivered by the pump. 4. Re-establish communication between the meter and pump by waiting for the pump display to timeout and then power up the meter. If the meter does not connect to the pump, the meter can be reset by holding the power button for 5 seconds. 5. Make sure you do not program a duplicate bolus. But if the original bolus amount was not delivered by the pump, program the undelivered bolus amount.

14 Glossary

Term	Definition
Acting time	The period of time from the start of a bolus until your blood glucose level is expected to return to the target level.
Active insulin	A calculated value representing the effective amount of insulin currently in the body that is working to lower blood glucose. This amount does not include any insulin that is working to account for carbohydrate intake. It also does not include basal insulin.
Advice options	Factors that influence bolus advice recommendations including meal rise, snack size, acting time and offset time.
After high bG reminder	A reminder to retest your blood glucose. When enabled, this reminder occurs after a high blood glucose result.
After low bG reminder	A reminder to retest your blood glucose. When enabled, this reminder occurs after a low blood glucose result.
After meal reminder	A reminder to retest your blood glucose. When enabled, this reminder occurs after a meal. For this reminder to occur, you must enter the meal time of a blood glucose test as before meal.

Term	Definition
Alarm	Audible or vibrating (silent) notification indicating a reminder, warning, error or maintenance message.
am	Ante Meridiem (12-hour clock notation for “before noon”)
Basal rate	The amount of insulin delivered per hour that is required to cover your basal, meal-independent insulin needs.
BE	Bread Equivalent
bG test reminders	Reminders to retest your blood glucose after a high blood glucose result, after a low blood glucose result or after a meal.
bG threshold	A bG test reminder setting; the upper limit is for your blood glucose for a high bG test reminder and the lower limit is for your blood glucose for a low bG test reminder.
Blood glucose (bG)	The level of glucose (sugar) in blood.

Term	Definition
Bluetooth Wireless Technology	Wireless short-range communications technology which connects devices (such as meter and pump) in order to exchange information.
Bolus	The amount of insulin delivered (in addition to the basal rate) to cover the intake of food and to correct high blood glucose levels. The bolus amount is determined by your healthcare professional's guidelines, your blood glucose level, your food intake, your activity level and other factors.
Bolus advice	When enabled, bolus advice provides a suggestion of how much insulin should be delivered for a meal and/or to correct for a blood glucose level.
ºC	Degrees Celsius (or Centigrade)
Carbohydrate (or Carb) ratio	The amount of insulin necessary to account for a certain amount of carbohydrates.

Term	Definition
Carbohydrates (or Carbs)	Carbohydrates include sugars and starches. Carbohydrates can increase blood glucose levels slowly or rapidly. Carbohydrates are generally counted to calculate a bolus insulin amount.
CC	Carbohydrate Choice
Control result	Value displayed on meter as the result of a control test. When the control result is within the range shown on the label of the test strip container, the test strips and the meter are working properly.
Control test	A meter test using control solution which lets you know that the meter and test strips are working properly.
Corrupt result	A historical result that cannot be displayed by the meter because of an error.
Current time	The time you set through the Settings menu and then in the Date and Time screen.
Default	The initial settings on the meter before you change or customise them.

Term	Definition
Delayed amount	The amount of insulin delivered over a period of time by an Extended Bolus or after the initial amount of a Multiwave Bolus.
Delayed duration	The amount of time over which an Extended Bolus or Multiwave Bolus is delivered.
Delivery speed	The speed at which the immediate amount of a Standard Bolus or Multiwave Bolus is delivered.
Discovery mode	When your meter or pump is “discoverable,” other Bluetooth devices can detect it, pair with it or connect to it.
Dismiss	Ends a reminder.
End time	The end time of a time block.
Extended bolus	A bolus delivered over a period of time. It can be helpful during long meals or when you have meals that are digested slowly. The Extended Bolus may also be appropriate for people who have gastroparesis (delayed digestion).

Term	Definition
FCC	Federal Communications Commission (United States)
Flight mode	This setting disables all wireless communication on the meter to comply with regulations on air travel.
g	Grams
GHz	Gigahertz
Health event	Information about your current health status or activities (Exercise 1, Exercise 2, Stress, Illness, Premenstrual or Customized). Up to 4 health events can be selected and stored with a blood glucose result. Each status or activity (health event) accounts for a certain percentage according to your settings and is used to adjust bolus advice recommendations.

Term	Definition
HI	Appears on the meter's screen when the test result is above the meter's measuring range.
Hyper	Hyperglycaemia: A condition that occurs when the blood glucose level is too high.
Hyper warning limit	A limit set in the meter. When your blood glucose result is above the hyper warning limit, a warning is displayed. The hyper warning limit should be provided by or discussed with your healthcare professional.
Hypo	Hypoglycaemia: A condition that occurs when the blood glucose level is too low.
Hypo warning limit	A limit set in the meter. When your blood glucose result is below the hypo warning limit, a warning is displayed. The hypo warning limit should be provided by or discussed with your healthcare professional.
IC	Industry Canada
Immediate amount	The amount of insulin delivered by a standard bolus or delivered at the beginning of a multiwave bolus.

Term	Definition
Insulin increment	The amount in units (U) by which your insulin dose is adjusted when programming a bolus or when entering a manual logbook entry.
Insulin pump	A device that can deliver a continuous supply of insulin into the body.
Insulin sensitivity	The amount of insulin necessary to lower your blood glucose by a certain amount.
ISO	International Organization for Standardization
KE	Kohlenhydrateinheit (carbohydrate unit)
Key lock	A function which disables the keys of a device in order to prevent its unintended use.
Lag time	The amount of time before a programmed bolus begins to be delivered.
Lanyard	A cord worn around the wrist or neck to carry an object.

Term	Definition
LCD	Liquid Crystal Display
LO	Appears on the meter's screen when the test result is below the meter's measuring range.
Manual on pump bolus	A bolus which is delivered by using the controls on the pump instead of the meter.
Max bolus	Max bolus serves as a safety measure against unintended large boluses. It is a setting on both the meter and pump that specifies a maximum bolus amount. For pen/syringe boluses, a bolus that is larger than the max bolus amount requires an additional confirmation. On the pump, no bolus larger than the max bolus amount can be delivered.
Meal rise	The increase in blood glucose levels during or after meals that is considered normal within a certain range, even though a bolus has been delivered.
Meal time	Information about the point in time of a blood glucose result (before meal, after meal, bedtime, fasting or other). It can be selected from a pop-up menu and is stored with a blood glucose result.
Meter	Blood glucose meter

Term	Definition
mmol/L	Millimoles per Litre
Multiwave bolus	Combines an immediate bolus delivery followed by an Extended Bolus delivery. A multiwave bolus can be helpful when you have meals that include both rapidly and slowly absorbed carbohydrates.
Mute	Temporarily silences a pump reminder. The reminder will recur in 60 seconds unless you select Dismiss.
N/A	Not Applicable
Note	Additional information
Offset time	The amount of time before the insulin begins to lower blood glucose levels.
Paired	Meter and another device exclusively communicate and transfer information with each other when they are paired. Pump and meter exclusively communicate and transfer information with each other when they are paired.
Pen/syringe bolus	A bolus delivered using a pen or syringe.

Term	Definition
PIN	Personal Identification Number
pm	Post Meridiem (12-hour clock notation for “after noon”)
Pump	See Insulin pump.
Quick bolus	A bolus delivery on the pump using the pump Quick Bolus keys. One key press equals one bolus increment (i.e., 0.1, 0.2, 0.5, 1.0 or 2.0 units of insulin). See the pump User’s Manual for more information.
Quick Notes	A logbook entry that can quickly be saved from the Main Menu or Status screen.
Remind after	A bG test reminder setting. The amount of time after a high blood glucose result, after a low blood glucose result or after a meal you want the reminder to occur.
Reminder	When enabled, reminders occur to remind you to test your blood glucose, to retest your blood glucose, or of an event or activity.

Term	Definition
RF	Radio Frequency
SD	Standard Deviation
Signal suspension	Suspends meter signals until the suspension period ends or the meter is turned on.
Snack size	The snack size defines a threshold of carbohydrates above which a meal rise is triggered.
Snooze	Reschedules a meter reminder to reoccur in a preset amount of time (for example, in 5 minutes).
Standard bolus	A bolus that is immediately delivered.
Standard deviation	As it is used in this User's Manual, standard deviation measures how widely spread the blood glucose results are (e.g., if the bG results are close to the bG average, then the standard deviation is small).

Term	Definition
Start time	The start time of a time block.
Target range	The desired upper and lower limits of your blood glucose level considered acceptable when fasting or before a meal as set by your healthcare professional.
Test strip	A plastic strip that, when inserted into a meter, reacts with a blood drop to deliver a blood glucose result.
Time block	One of up to eight time periods within one day.
Time scale	The user sets the duration of time to configure a My Data graph or table.
Touchscreen	A screen that can be touched to interact with the device.
U	Units (insulin units)
USB	Universal Serial Bus
Warning	Describes items and conditions that present hazards and may cause personal injury.

Term	Definition
Warning limit	See Hyper warning limit or Hypo warning limit.

Index

A

acting time
  description 28
  setting 21
automatic off timer 128

B

basal profile
  activating 107
  clearing 109
  programming 103
basal rate
  basic temporary basal rate 93
  cancelling 98
  customised temporary basal rate 95
  deleting 100
battery 206
blood glucose
  adding information 52
  result 50, 52
  testing 47
blood glucose result, detailed bG result 51
bolus
  cancelling a bolus 82, 84
  deleting a customised bolus 80
  delivering 55
  settings 130, 132, 133, 134, 135
  type 56
bolus advice
  options 28
  overview 25
  setting up 18
bolus delivery 69
  custom 76
  extended 60, 72
  manual on pump 67
  multiwave 62, 74
  pen/syringe 65
  standard 57, 70
  using bolus advice 86

C

carbohydrate
  set amount 163, 167
  unit description 22
  unit setting 18
carbohydrate ratio
  description 26
  setting 19
carbohydrates accepted icon 158
carbohydrates not accepted icon 159
cartridge warning level 139
charging the battery 9
communication 31
communication lost 208

D

date and time 18, 115, 150
delivery speed 133
device not paired 206, 207
device settings 115, 141

F

flight mode 113, 114

H

health events
  choose health event 53, 163, 168
  setting percentages 21
home screen, description 5
hyper warning limit 18
hypo warning limit 18

I

icon list 156, 201
information message 206, 207
infusion set
  change reminder 122
  settings 137
insulin sensitivity
  description 26
  setting 19

K

key lock 146

L

lag time 135
language 17
logbook
  adding new data 166
  adjusting data 161
  description 154
  record description 154

M

main menu screen 6
maintenance message 207, 208
maximum bolus amount 134
meal rise
  description 28
  setting 21
meal time 53, 163, 167
my data 153

N

no devices found 206

O

offset time
  description 29
  setting 21

P

pairing 31
pump language 148
pump reminders 115, 116, 117
pump settings 115

Q

quick bolus increment 132

S

scroll bar 6
setup wizard 14, 16
signal mode 111, 141, 144
signal suspension 144
snack size
  description 28
  setting 21
splash screen 16
status screen 7
symbols 200

T

target range 19
test strip container 47
test strip slot 48
therapy settings 115, 127
time 18
time blocks 24
time format 17
trend graph 170

U

USB
  cable 9, 12
  PC port 12
use by date 47

W

warning limits
  description 23
  setting 18

Distributed in the United Kingdom by:
Roche Diabetes Care Limited
Charles Avenue, Burgess Hill
West Sussex, RH15 9RY, **United Kingdom**
Accu-Chek Pump Careline [1]:
UK Freephone number: 0800 731 22 91
ROI Freephone number: 1 800 88 23 51
[1] calls may be recorded for training purposes
Some mobile operators may charge for calls to these numbers.
burgesshill.insulinpumps@roche.com
www.accu-chek.co.uk
www.accu-chek.ie

© 2018 Roche Diabetes Care

ACCU-CHEK, ACCU-CHEK 360°, ACCU-CHEK AVIVA, ACCU-CHEK INSIGHT and ACCU-CHEK AVIVA INSIGHT are trademarks of Roche.

CONTINUA, the CONTINUA logos and CONTINUA CERTIFIED are trademarks, service marks, or certification marks of the Continua Health Alliance. CONTINUA is a registered trademark in some, but not all countries in which this product is distributed.

The *Bluetooth*® word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. and any use of such marks by Roche is under license.

All other product names and trademarks are the property of their respective owners.

Roche Diabetes Care GmbH
Sandhofer Strasse 116
68305 Mannheim, Germany
www.accu-chek.com

CE 0088

Last Update: 2017-08

07046553001/F